


Applied Computational Electromagnetics Society Journal

Special Issue on
Phased and Adaptive
Array Antennas

Guest Editor
Deb Chatterjee

November 2006
Vol. 21 No. 3
ISSN 1054-4887

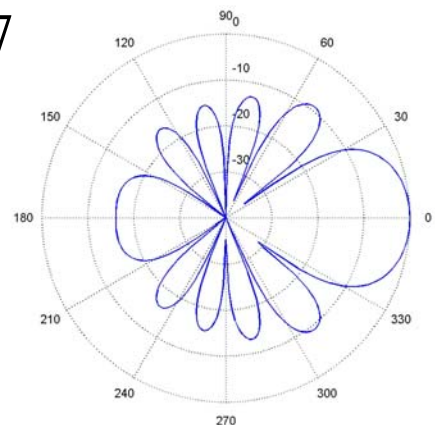

GENERAL PURPOSE AND SCOPE: The Applied Computational Electromagnetics Society (*ACES*) Journal hereinafter known as the *ACES Journal* is devoted to the exchange of information in computational electromagnetics, to the advancement of the state-of-the art, and the promotion of related technical activities. A primary objective of the information exchange is the elimination of the need to “re-invent the wheel” to solve a previously-solved computational problem in electrical engineering, physics, or related fields of study. The technical activities promoted by this publication include code validation, performance analysis, and input/output standardization; code or technique optimization and error minimization; innovations in solution technique or in data input/output; identification of new applications for electromagnetics modeling codes and techniques; integration of computational electromagnetics techniques with new computer architectures; and correlation of computational parameters with physical mechanisms.

SUBMISSIONS: The *ACES Journal* welcomes original, previously unpublished papers, relating to applied computational electromagnetics. Typical papers will represent the computational electromagnetics aspects of research in electrical engineering, physics, or related disciplines. However, papers which represent research in applied computational electromagnetics itself are equally acceptable.

Manuscripts are to be submitted through the upload system of *ACES* web site <http://aces.ee.olemiss.edu> See “Information for Authors” on inside of back cover and at *ACES* web site. For additional information contact the Editor-in-Chief:

Dr. Atef Elsherbeni

Department of Electrical Engineering
The University of Mississippi
University, MS 386377 USA
Phone: 662-915-5382 Fax: 662-915-7231
Email: atef@olemiss.edu

SUBSCRIPTIONS: All members of the Applied Computational Electromagnetics Society who have paid their subscription fees are entitled to receive the *ACES Journal* with a minimum of three issues per calendar year and are entitled to download any published journal article available at <http://aces.ee.olemiss.edu>.

Back issues, when available, are \$15 each. Subscriptions to *ACES* are through the web site. Orders for back issues of the *ACES Journal* and changes of addresses should be sent directly to *ACES* Executive Officer:

Dr. Richard W. Adler

ECE Department, Code ECAB
Naval Postgraduate School
833 Dyer Road, Room 437
Monterey, CA 93943-5121 USA
Fax: 831-649-0300
Email: rwa@attglobal.net

Allow four week’s advance notice for change of address. Claims for missing issues will not be honored because of insufficient notice or address change or loss in mail unless the Executive Officer is notified within 60 days for USA and Canadian subscribers or 90 days for subscribers in other countries, from the last day of the month of publication. For information regarding reprints of individual papers or other materials, see “Information for Authors”.

LIABILITY. Neither *ACES*, nor the *ACES Journal* editors, are responsible for any consequence of misinformation or claims, express or implied, in any published material in an *ACES Journal* issue. This also applies to advertising, for which only camera-ready copies are accepted. Authors are responsible for information contained in their papers. If any material submitted for publication includes material that has already been published elsewhere, it is the author’s responsibility to obtain written permission to reproduce such material.

APPLIED COMPUTATIONAL ELECTROMAGNETICS SOCIETY JOURNAL

Special Issue on
Phased and Adaptive Array Antennas

Guest Editor
Deb Chatterjee

November 2006
Vol. 21 No. 3

ISSN 1054-4887

The ACES Journal is abstracted in INSPEC, in Engineering Index, and in DTIC.

The first, fourth, and sixth illustrations on the front cover have been obtained from the Department of Electrical Engineering at the University of Mississippi.

The third and fifth illustrations on the front cover have been obtained from Lawrence Livermore National Laboratory.

The second illustration on the front cover has been obtained from FLUX2D software, CEDRAT S.S. France, MAGSOFT Corporation, New York.

THE APPLIED COMPUTATIONAL ELECTROMAGNETICS SOCIETY

<http://aces.ee.olemiss.edu>

ACES JOURNAL EDITORS

EDITOR-IN-CHIEF/ACES/JOURNAL

Atef Elsherbeni

University of Mississippi, EE Dept.
University, MS 38677, USA

EDITORIAL ASSISTANT

Matthew J. Inman

University of Mississippi, EE Dept.
University, MS 38677, USA

EDITOR-IN-CHIEF, EMERITUS

David E. Stein

USAF Scientific Advisory Board
Washington, DC 20330, USA

ASSOCIATE EDITOR-IN-CHIEF

Alexander Yakovlev

University of Mississippi, EE Dept.
University, MS 38677, USA

EDITOR-IN-CHIEF, EMERITUS

Ducan C. Baker

EE Dept. U. of Pretoria
0002 Pretoria, South Africa

EDITOR-IN-CHIEF, EMERITUS

Allen Glisson

University of Mississippi, EE Dept.
University, MS 38677, USA

MANAGING EDITOR

Richard W. Adler

833 Dyer Rd, Rm 437 EC/AB
NPS, Monterey, CA 93943-5121, USA

EDITOR-IN-CHIEF, EMERITUS

Robert M. Bevensee

Box 812
Alamo, CA 94507-0516, USA

EDITOR-IN-CHIEF, EMERITUS

Ahmed Kishk

University of Mississippi, EE Dept.
University, MS 38677, USA

ACES JOURNAL ASSOCIATE EDITORS

Giandomenico Amendola

Universita' della Calabria
Rende , Italy

John Beggs

NASA Langley Research Center
Hampton, VA, USA

Malcolm Bibby

Gullwings
Weston, MA , US

John Brauer

Ansoft Corporation
Milwaukee, WI, USA

Magda El-Shenawee

University of Arkansas
Fayetteville AR, USA

Pat Foster

Microwave & Antenna Systems
Gt. Malvern, Worc. UK

Cynthia M. Furse

Utah State University
Logan UT, USA

Christian Hafner

Swiss Federal Inst. of Technology
Zurich, Switzerland

Michael Hamid

University of South Alabama,
Mobile, AL, USA

Andy Harrison

Radiance Technologies, Inc.
Huntsville, AL

Chun-Wen Paul Huang

Anadigics, Inc.
Warren, NJ, USA

Todd H. Hubing

University of Missouri-Rolla
Rolla, MO, USA

Nathan Ida

The University of Akron
Akron, OH, USA

Yasushi Kanai

Niigata Institute of Technology
Kashiwazaki, Japan

Leo C. Kempel

Michigan State University
East Lansing MI, USA

Andrzej Krawczyk

Institute of Electrical Engineering
Warszawa, Poland

Stanley Kubina

Concordia University
Montreal, Quebec, Canada

Samir F. Mahmoud

Kuwait University
Safat, Kuwait

Ronald Marhefka

Ohio State University
Columbus, OH, USA

Edmund K. Miller

LASL
Santa Fe, NM, USA

Krishna Naishadham

Wright State University
Dayton, OH, USA

Giuseppe Pelosi

University of Florence
Florence, Italy

Vicente Rodriguez

ETS-Lindgren
Cedar Park, TX, USA

Harold A. Sabbagh

Sabbagh Associates
Bloomington, IN, USA

John B. Schneider

Washington State University
Pullman, WA, USA

Amr M. Sharawee

American University
Cairo, Egypt

Norio Takahashi

Okayama University
Tsushima, Japan

Guest Editorial

ACES Invited Special Issue on *Phased and Adaptive Array Antennas*

This *invited* special issue of the Applied Computational Electromagnetics Society (ACES) Journal on *Phased and Adaptive Array Antennas* aims to capture information on a broad spectrum of the various aspects involved in array radiating systems and their applications. Recent advances in this area can be found in [1]-[3]. The earlier special issue [4] on a closely similar topic served as a guide in preparing for this ACES special issue. The information gleaned from these sources resulted in a widening of the scope of this special issue than was originally planned. For enhanced impact, it appeared appropriate to solicit contributions from leading researchers in the antennas and computational electromagnetics (CEM) areas. To that end, in quite a few cases, the topic of the invited contribution was suggested to the individual authors. All invited papers were peer-reviewed per standard guidelines.

In all there are twenty papers co-authored or authored by leading researchers from various countries. They represent a wide range of topics on phased and adaptive arrays. Specifically, papers on characteristic basis functions, genetic algorithms, ship-board arrays, conformal arrays, phased arrays for biomedical applications, multiple-beam phased arrays, array mutual coupling compensation, power-divider network, etc., appear here and provide useful information on both modeling and practical applications of phased and adaptive arrays. The valuable contribution of the authors and their patience is gratefully acknowledged.

In the course of assembling the special issue, special thanks go to Prof. Atef Elsherbeni (editor-in-chief) and Prof. Alexander Yakovlev (associate editor-in-chief) of ACES Journal, University of Mississippi (Ole Miss). The encouragement from Dr. W. Ross-Stone, editor-in-chief, *IEEE Antennas and Propagation Magazine*, is deeply appreciated. It is a pleasure to acknowledge the extensive editorial help from Mr. Mohamed Al Sharkawy (Ole Miss), in the final stages. At University of Missouri Kansas City (UMKC), Mr. Naresh Vijaya Yalamanchili had painstakingly retyped some of the manuscripts for this invited special issue. Thanks to all of them for their continued encouragement and timely help. Without their active support this endeavor would not have come to fruition.

The final judgment on the quality of this invited special issue rests on the reader. It is hoped that the reader shall find the contents in these papers of continuing value. Any drawback or other errors is the sole responsibility of the guest editor.

References

- [1] Arun K. Bhattacharyya, *Phased Array Antennas: Floquet Analysis, Synthesis, BFNs, and Active Array Systems*. Hoboken, NJ, USA: John-Wiley & Sons, Inc., 2006.
- [2] L. Josefsson and P. Persson, *Conformal Array Antenna: Theory and Design*. Hoboken, NJ, USA: Wiley-Interscience, 2006.
- [3] L. C. Godara, *Smart Antennas*. Boca Raton, FL, USA: CRC Press, 2004.
- [4] R. J. Mailloux (ed.), Special Issue on *Phased Arrays*, IEEE Transactions on Antennas and Propagation, vol. 47, no. 3, March 1999.



Deb Chatterjee is an associate professor of Electrical and Computer Engineering, with the Computer Science and Electrical Engineering (CSEE) Department at University of Missouri Kansas City (UMKC), where he joined as a faculty in August 1999. He obtained his M.A.Sc. and Ph.D. degrees in Electrical and Computer Engineering and Electrical Engineering, from Concordia University, Montreal, Canada and University of Kansas, Lawrence, Kansas, respectively. His current research interests are in phased arrays, high-frequency scattering and propagation, miniature, ultra-wideband microstrip antennas. He has served as a reviewer of technical articles for *IEEE Transactions on Antennas and Propagation*, *IEEE Antennas and Wireless Propagation Letters*, *Radio Science*, and the *Applied Computational Electromagnetics Society (ACES) Journal*. Currently he serves as an associate editor for *International Journal of Antennas and Propagation (IJAP)*. Dr. Chatterjee has published 35 articles in peer-reviewed journals and conference proceedings, and has taught courses in the area of electromagnetics and antennas at undergraduate and graduate levels. He is a member of the IEEE Antennas and Propagation and the Applied Computational Electromagnetics Societies.

THE APPLIED COMPUTATIONAL ELECTROMAGNETICS SOCIETY
JOURNAL

Vol. 21 No. 3

November 2006

TABLE OF CONTENTS

"A Hybrid Framework for Antenna/Platform Analysis "	
R. J. Burkholder, P. H. Pathak, K. Sertel, R. J. Marhefka, J. L. Volakis, and R. W. Kindt .	177
"Low SAR Phased Antenna Array for Mobile Handsets "	
J. Moustafa, N. J. McEwan, R. A. Abd-Alhameed, and P. S. Excell	196
"Numerical Simulation Approaches for Phased Array Design"	
L. Sevgi	206
"Modeling Large Phased Array Antennas Using the Finite Difference Time Domain Method and the Characteristic Basis Function Approach"	
N. Farahat, R. Mittra, and N. Huang.....	218
"Direction of Arrival Estimation in a Multipath Environment: an Overview and a New Contribution"	
E. M. Al-Ardi, R. M. Shubair, and M. E. Al-Mualla	226
"Polarization Isolation Characteristics Between Two Center-Feed Single-Layer Waveguide Arrays Arranged Side-by-Side"	
Y. Tsunemitsu, J. Hirokawa, M. Ando, Y. Miura, Y. Kazama, and N. Goto.....	240
"Radiation by a Linear Array of Half-Width Leaky-Wave Antennas"	
D. Killips, J. Radcliffe, L. Kempel, and S. Schneider.....	248
"Macro-Scale Basis Functions for the Method of Moment Analysis of Large Periodic Microstrip Arrays"	
A. Cucini and S. Maci.....	256
"A Serial-Parallel FDTD Approach for Modeling the Coupling problem between Two Large Arrays"	
R. Mittra, H. E. Abd-El-Raouf, and N. Huang.....	267
"Preconditioned GIFFT: A Fast MoM Solver for Large Arrays of Printed Antennas"	
B. J. Fasenfest, F. Capolino, and D. R. Wilton.....	276
"Generalized Scattering Matrix (GSM) Approach for Multilayer Finite Array Analysis"	
A. K. Bhattacharyya.....	284

"Modeling the RF Performance of a Small Array" P. R. Foster and A. E. Wicks.....	291
"A Critical Examination of Receive and Transmit Scan Element Pattern for Phased Arrays" R. C. Hansen.....	299
"Modeling Conformal Array Antennas of Various Shapes Using Uniform Theory of Diffraction (UTD)" P. Persson	305
"Efficient Wideband Power Divider for Planar Antenna Arrays" V. Demir, D. A. Elsherbeni, D. Kajfez, and A. Z. Elsherbeni	318
"Genetic Algorithm Applications for Phased Arrays" R. L. Haupt	325
"Genetic Algorithm Optimization of a Traveling Wave Array of Longitudinal Slots in a Rectangular Waveguide" A. Jensen and S. R. Rengarajan.....	337
"Approximate Compensation for Mutual Coupling in a Direct Data Domain Least Squares Approach using the In-situ Measured Element Patterns " W. Choi, T. K. Sarkar, O. E. Allen, and J. S. Asvestas.....	342
"Multiple Beam Antenna Technology for Satellite Communications Payloads" S. Rao, M. Tang, and C. Hsu.....	353
"A Survey of Phased Arrays for Medical Applications" C. Furse	365

A Survey of Phased Arrays for Medical Applications

(Invited Paper)

Cynthia Furse

Electrical and Computer Engineering, University of Utah, 50 S Campus Drive 3280 MEB
Salt Lake City, Utah 84112

cfurse@ece.utah.edu, www.ece.utah.edu/~cfurse

Phone: (801) 585-7234

Fax: (801) 581-5281

Abstract—This paper presents a survey of phased arrays for a wide variety of medical applications. Medical imaging modalities including tomography, confocal imaging, thermography, and MRI are covered, as well as hyperthermia for treatment of cancer. Arrays include planar, cylindrical, and conformal configurations of many types of antennas including monopoles, dipoles, microstrips, horns, bowties, loops, etc.

Keywords—Antenna Arrays, Medical Imaging, Breast Cancer, Hyperthermia, Magnetic Resonance Imaging (MRI)

I. INTRODUCTION

Antenna arrays have been used for a wide variety of medical applications, most notably imaging and hyperthermia treatment of cancer. These arrays may be phased electronically; however more often the received signals are phased after detection. The arrays can be built of multiple antennas or can be produced synthetically by scanning a single antenna or pair of antennas over the object of interest. Medical applications for phased arrays have borrowed heavily on radar applications such as ground penetrating radar, ultrawideband radar, and synthetic aperture radar. This paper surveys the medical imaging and hyperthermia applications of phased array antennas. Microwave tomography, confocal imaging, thermography, and magnetic resonance imaging are covered in section II. Hyperthermia is covered in section III. Some numerical methods for simulating antenna arrays are surveyed in section IV.

II. ANTENNA ARRAYS FOR MEDICAL IMAGING

One of the most promising uses of antenna arrays in medical applications is for imaging the location of leukemia 0, breast tumours [1] - [25], and cardiac anomalies [26] - [27]. Microwave imaging methods rely on the fact that the electrical properties of normal

and malignant tissue are significantly different [28] - [35] and that there is significant variation from tissue to tissue. Location of breast cancer shows particular promise, because the relatively low loss of fatty tissue allows electromagnetic fields to propagate to the tumor and back, and the proximity of the tumor to the outer surface of the body means that the signal does not have more than a few inches to propagate. Two major microwave imaging methods utilize antenna arrays. Tomography [2] - [9] attempts to map a complete electrical profile of the breast, and confocal imaging [10] - [25] maps only the location of significant scatterers. Both of these methods have used antenna arrays made up of wideband elements to send and receive the test signals. Microwave thermography picks up the passive electromagnetic fields from the body [36] - [52]. Magnetic Resonance Imaging (MRI) uses a strong magnetic field to cause the magnetic dipoles in the body to align and precess, gradient fields to control and tip the dipoles and then uses an array of receiving loops to pick up the fields when they relax back to their normal state [59] - [74].

A. Tomography for Breast Cancer Detection

Microwave tomography is used to provide a complete spatial mapping of the electrical properties in the region of interest. During the acquisition phase, an array of antennas surrounds the region of interest. One of the antennas in the array is used to transmit a signal, normally a sine wave [2], set of sine waves [3] - [4], or a broadband signal [5], and all of the other antennas are used to receive the reflected signal. The array is scanned so that each antenna transmits each frequency, and those signals are received by each of the other antennas. After all of the data has been acquired, it is processed by comparing the received data with what would be expected from a simulated model of the region. A numerical “forward model” is used to predict how much power is transmitted from the transmit antenna, passes into and reflects from the breast/tumor model, and is received by the receive antenna. Originally the simulated model is just a good guess for

what might be present, generally a generic breast model with no tumor. The differences between the measured and expected received data are used to modify the original guess to obtain an ideal model that best matches the measured data. This “inversion” is used to predict what model would have produced the measured data.

Microwave tomography for breast cancer has been demonstrated by several groups [2] - [9]. In the Dartmouth system, [2] for instance, sine waves from 300-1000 MHz (being expanded to 3 GHz) are transmitted from a circular array of 16 transmit/receive monopole antennas to produce 2D reconstructed images of the breast. Quarter wave monopole antennas (in the fluid) were built by extending the inner conductor of semi-rigid coax used for this application. Monopoles were chosen, because they are easy to model as a line source in a 2D reconstruction algorithm with high accuracy [2]. Water-filled waveguide apertures have also been used for tomography, however the monopole antennas were found to be as accurate, and easier to build [6]. The accuracy of the tomography approach depends on being able to accurately predict the expected received fields from a given transmit antenna / breast model. The antennas and their locations must be accurately modeled in both the transmit and receive case, as any inaccuracy in the antenna models affect the forward model not once, but twice and has a significant impact on the accuracy of the final solution. Monopole antennas can be very accurately modeled and are a good choice for this application. In addition, monopoles have been found to be excellent radiators when resistively loaded by lossy material, having a return loss of about -10 dB from 100 to 1100 MHz when immersed in saline [6]. Thus, for applications such as medical imaging where it is imbedded in a lossy conducting fluid surrounding the object of interest, simple monopoles demonstrate good radiation properties [2]. One of the key factors in obtaining accurate models of the antenna array is to model each of the inactive array elements as a microwave sink, so that the signal is not re-radiated [7] -[8]. This was accomplished in the numerical model by imposing an impedance boundary condition on a finite diameter around each inactive element. The forward model uses a hybrid boundary element (BEM) and finite element method (FEM). In the hardware, a matched switch was the last element in the switching matrix, so that when the antenna is not radiating, any coupled signal is terminated at the switch. The 32 channel data acquisition system allows each antenna (16 transmit and 16 receive) to act as only a transmitter or receiver, which provides a dynamic range of 130 dB and channel-to-channel isolation of greater than 120 dB.

Since the goal is to identify tumours that have significant dielectric discontinuity from the surrounding

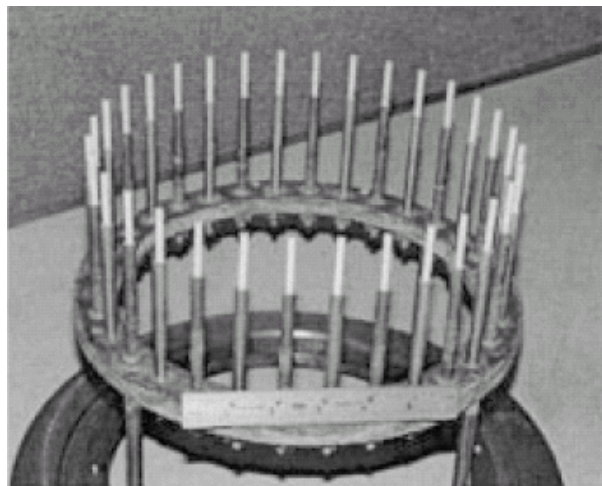


Fig. 1. 2D Monopole array used for tomographic imaging of the breast (from [2] © 2000 IEEE).

tissue, best results will be obtained if they are the primary scatterers in the environment. Blood vessels are also significant scatterers, but these cannot be controlled. They will also show up on a tomographic image. The other major scattering source is the air-skin interface, and this can be controlled. This reflection can be minimized by immersing the antennas and breast in a fluid medium that is electrically similar to breast/skin. Originally saline was used, which is a better match than air, inexpensive and safe, however its relative permittivity is significantly higher than that of fatty breast tissue, and a better matched fluid material is recommended. The monopole antennas are designed to be used in the liquid medium, rather than air, with the conductive fluid providing the resistive loading of the monopoles. The feed system also needs to be designed so that it can be used in fluid. The sealing of the antenna feed system along with the ability to raise and lower the array in parallel with the fluid level was a significant challenge in the system prepared for clinical trials in [6].

For a microwave tomography breast exam, the woman lies with the breast pendant through a hole in the examination table and immersed in the tank of matching fluid. The circuit antenna array of monopoles is also immersed in this fluid and radially surrounds the breast. For each 2D breast scan, signals are transmitted from each antenna and individually received in parallel at the remaining antennas. This is repeated for 12 frequencies over the 300-1000 MHz band. This is repeated for seven vertical array positions on the order of 1cm. The total acquisition time for the 3D image of both breasts is about 15 min. A complete set of seven images at a single frequency can be reconstructed in less than 5 min using a Compaq AlphaServer ES40 68/833.

Microwave tomography has been validated experimentally [9]. The presence of 1.1 or 2.5 cm saline tubes (representing tumours) in excised breast tissue are seen to be clearly visible [8]. Objects as small as 4 mm in diameter have been imaged at 900 MHz [9].

B. Confocal Imaging for Breast Cancer Detection

Confocal imaging for breast cancer detection is another exciting application of antenna arrays in medical imaging. Confocal imaging is similar to ground penetrating radar. Unlike microwave tomographic imaging, this method does not provide a complete electrical mapping of the region of interest. Instead it identifies locations of significant scattering. This method typically uses a single antenna scanned in a flat array pattern above the breast or in a cylindrical pattern around the breast [10]. For planar imaging, the patient lies face up, and the antenna is physically scanned in a plane above the breast [11] - [13]. For cylindrical imaging, the patient lies face down, with the breast extending into a cylindrical tank containing the antenna through a hole in the table [14] - [15]. Matching fluid surrounding the breast, similar to that used for microwave tomography, is suggested in this case. Both methods provide similar results [15]. The confocal imaging process is shown in Fig. 2. One antenna in the array transmits an ultrawideband pulse, which propagates into the breast, where it is reflected off significant electrical discontinuities, and is received in parallel by the other antennas in the array. Knowing the physical spacing between the array elements, the different delays between the transmit antenna, scattering point, and receiving antenna can be calculated geometrically. The received pulses representing a specific point in space can then be time delayed appropriately for each antenna, added up and integrated to indicate the magnitude of the scattered energy from that point in space. This is effectively correlating the signals received from that point at all antennas.

The antennas used for confocal imaging must be ultrawideband and small enough to fit within the relatively small array area. Resolution of less than 1 cm requires a bandwidth of at least 5 GHz. The lossy nature of tissue attenuates high frequency signals, limiting the upper frequency to about 10 GHz. Initially, resistively loaded bowtie were suggested for the planar configuration, [11]-[13], [17], [19], while dipole antennas were suggested for the cylindrical system [14]-[15]. Resistively loaded Vee dipoles have also been proposed [18]. In the cylindrical configuration, and the planar system, a single antenna is scanned over the surface, creating a synthetic antenna aperture. In order to overcome the inherent inefficiency of resistively loaded antennas, a modified ridged horn antenna

operating from 1 to 11 GHz has been introduced [20]. Most of the antennas are designed to observe co-polarized reflections from the breast, however using two resistively loaded bowtie antennas in the shape of a Maltese cross has also been proposed to pick up the cross polarized reflections[12]. Cross-polarized reflections from simple tumor models were also examined in [16].

The antenna shown in Fig. 3 [16] consists of two cross polarized bowtie antenna elements, an octagonal cavity behind the bowtie elements, and a metal flange attached to the cavity. The broadband bowties have flare angles of 45°. They are 1.67 cm long, which is a half-wavelength at 3 GHz in fat (similar to breast). The octagonal cavity blocks waves radiated away from the breast.

The cavity is approximated as a circular waveguide filled with fat material for matching and size reduction. The first cutoff frequency is set to be 2 GHz for 2-4 GHz operation. The cavity length is a quarter-wavelength, which is 11 mm at 3 GHz. The flange consists of an inner and outer component, and is designed to block unwanted waves such as surface waves. The antenna performance does not change significantly when the flange size is varied between 10–6.25 cm, therefore, the width of the outer flange is set to be 6.25 cm. The inner flange is designed to prevent possible electric field overshoot at the inner corners of the opening of the octagonal cavity or at the ends of the bowtie elements.

A slotline bowtie antenna shown in Fig. 4 has also been proposed in [22]. The slotline was produced on a high dielectric substrate (Rogers RT-Duroid 6010.2LM, Rogers Corporation, Rogers, CT, USA). The substrate has an ϵ_r of 10.2 at 10 GHz with a low-loss factor $\tan \delta$ of 0.0023 and a thickness of 635 μm . The ultrawideband balun uses a via as a short. The holes for the vias in the balun are drilled and electroplated. The balun and the profile of the antenna are then milled. The bowtie plates are designed to be cut from a 508 μm -thick sheet of copper. To obtain the correct contour of the plates accurately without damaging the fragile antenna board, a steel jig was made by tracing the contour of the antenna board. The bowtie plates were bent along this jig, and then carefully soldered on to the antenna board at right angles. The antenna plates were encased in a dielectric epoxy (Eccostock Hi K Cement, Emerson & Cuming Microwave Products, Randolph, MA, USA) with $\epsilon_r = 10$ for structural support and improved matching.

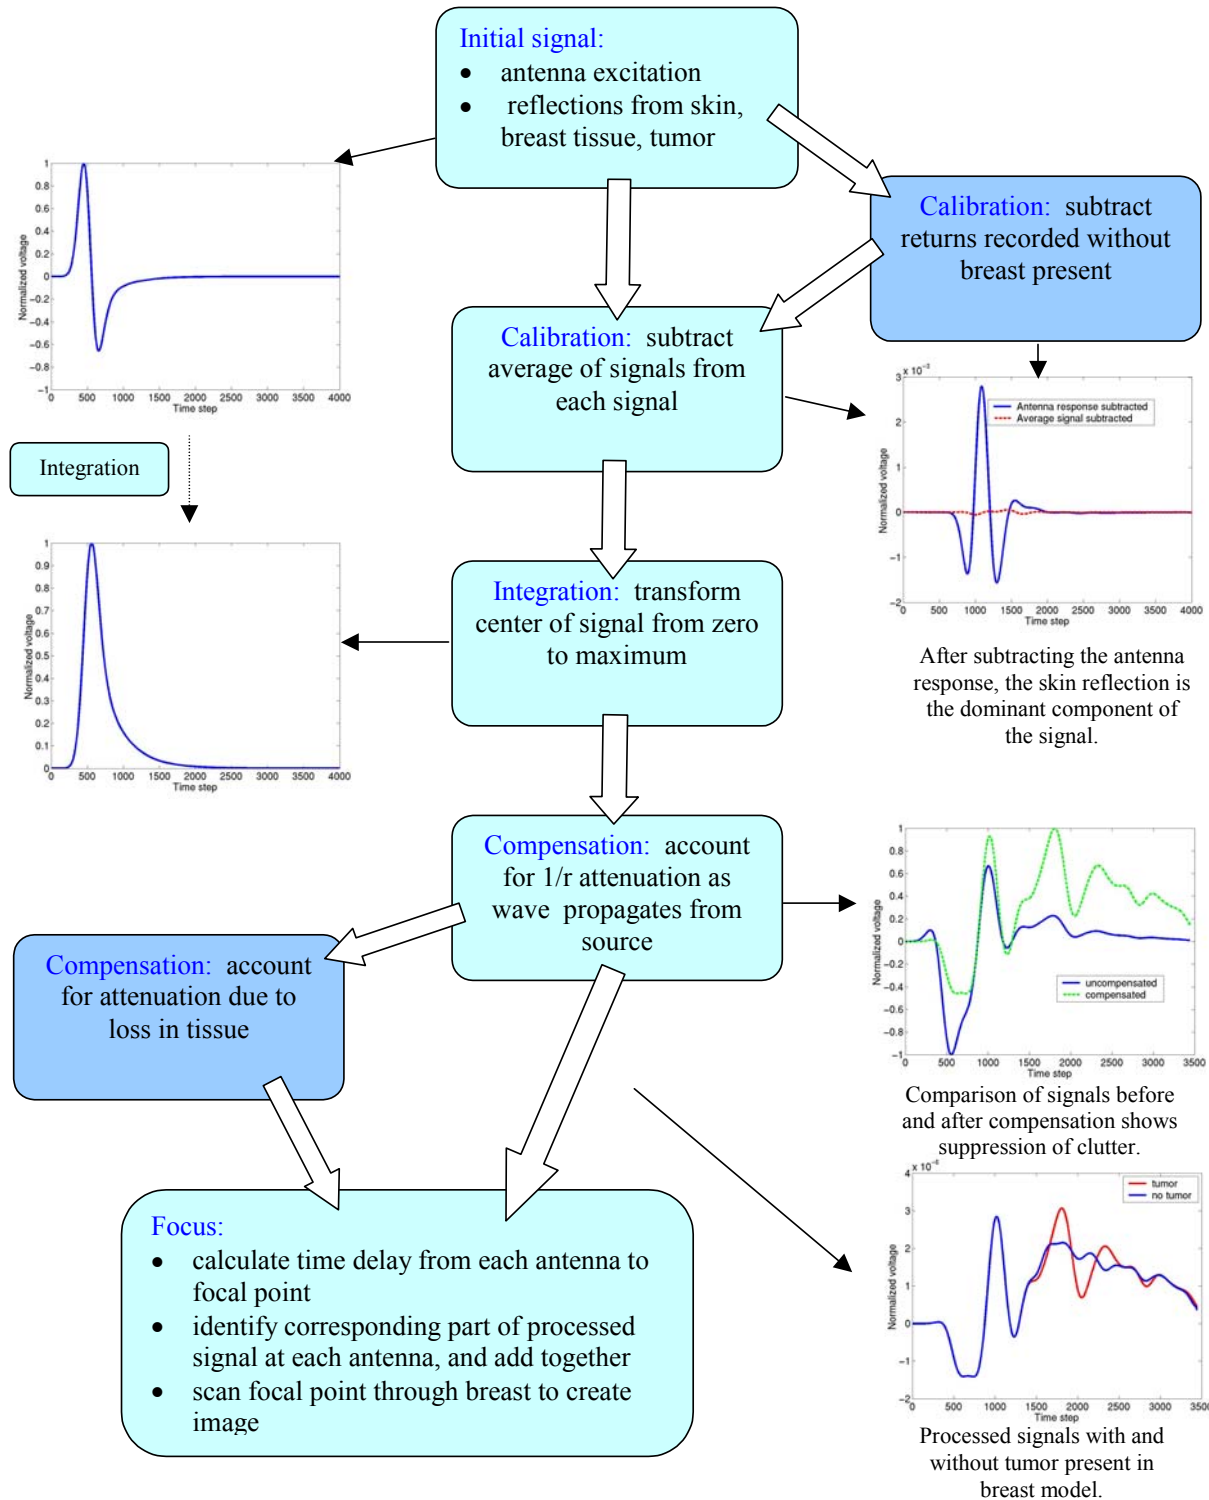


Fig. 2. Confocal Microwave Imaging Process. (From [10] © 2002 IEEE)

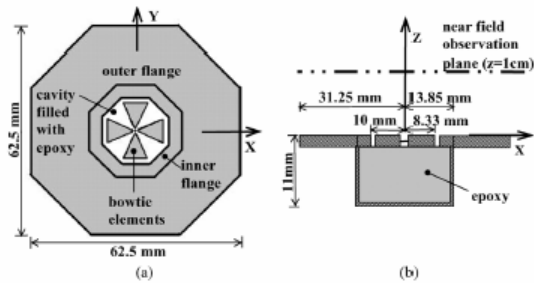


Fig. 3. Cross polarized antenna for confocal imaging. The properties of the substance inside the cavity and the medium outside the antenna are similar to fat ($\epsilon_r = 9$; $\sigma = 0.2$ S/m). (From [16] © 2005 IEEE)

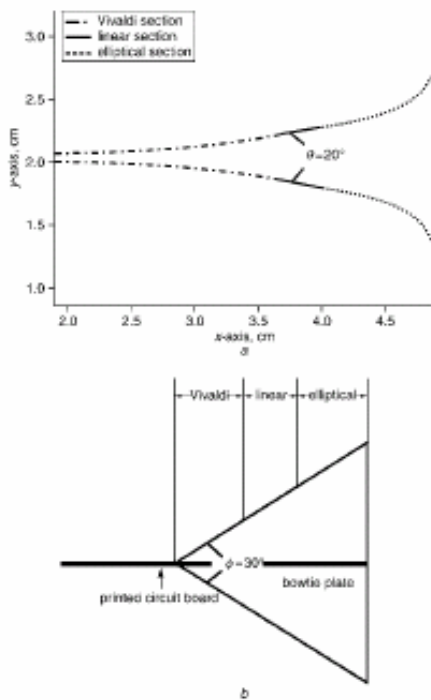


Fig. 4. Slotline Antenna and a Top view with Vivaldi, linear and elliptical sections indicated b Side view with Vivaldi, linear and elliptical sections and bowtie plates. (From [22] © 2005 IEEE)

A resistively loaded monopole antenna shown in Fig. 5 suitable for use in the cylindrical system was proposed in [25]. Based on the Wu-King design [75] - [76] this antenna was designed to be useable from 1to10 GHz immersed in canola oil ($\epsilon_r = 3.0$) for matching to breast tissue. The antenna is fabricated using high-frequency chip resistors (Vishay 0603HF) (Malvern, PA) soldered to a high-frequency substrate (Rogers RO3203 series) (Rogers Corporation, Chandler, AZ). The substrate ($\epsilon_r = 3.02$ and $\sigma = 0.001$ S/m) has electrical properties similar to those of the canola oil.

The antenna is soldered to a subminiature A (SMA) connector and attached to a metal plug for connection into the oil-filled test canister.

The cylindrical confocal imaging system has been experimentally tested [77], [23], [25]. Simulated tumours of diameter 1 cm have been detected using a system that represents the skin as 2D and the tumor model as 3D.

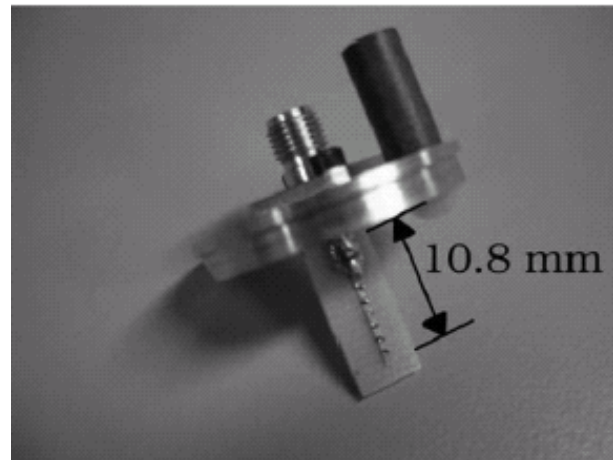


Fig. 5. Fabricated resistively loaded monopole antenna soldered to an SMA connector and attached to a metal plug. (From [25] © 2005 IEEE)

C. Microwave Radiometry

Microwave radiometry is a passive method where the natural electromagnetic radiation or emission from the body is measured to allow detection or diagnosis of pathogenic conditions in which there are disease-related potentials [36] -[37]. This method has been proposed for detection of breast cancer [40], [50], [51] and brain cancer [41], in which the metabolism of cancer cells increases the localized temperature 1-3°C. This method has also been used for fluid and blood warming [37], detection or rheumatology [39], and for monitoring of temperature rise during hyperthermia treatment [38].

Typical antennas include open ended rectangular waveguides [42]-[45], small-loop antennas [47], or a horn antenna with a dielectric lens [48]. Working around 3 GHz, all of these antennas have radiation patterns that have minimal penetration into the body, thus strongly weighting them to monitoring of surface temperatures. [49], [52] Increased focus and therefore better spatial accuracy was obtained with an array of six rectangular aperture antennas filled with low loss dielectric ($\epsilon_r = 25$), which were scanned over the object of interest in an overlapping pattern. Preliminary results indicated promise for location of breast tumours [50] - [51].

D. Magnetic Resonance Imaging

Magnetic Resonance Imaging (MRI) uses a very strong magnetic field (0.5T, 1.5T, 3T, 4T, 7T, perhaps in the future 8T) to make the magnetic dipoles in the body precess (line up). When they are released, a set of receiver coils picks up the magnetic field created when these dipoles return to their normal orientations (position may change a lot as in blood imaging, diffusion etc.). The relaxation properties of the different tissues effects the relative received signal intensities and a 3D map of the body can be produce. There are two basic types of receiver coils used for MRI. Volume coils, such as the quadrature birdcage head coil shown in Fig. 6 [53] and whole body coils [54] are used for imaging large and deep anatomic structures volume of the body and provide homogeneous field profiles.. For high resolution applications that are more localized, such as angiographic imaging, hippocampus imaging, and functional imaging, in which the object features are very small, volume coils pick up less signal and more noise, thus having a lower signal to noise ratio and poor quality images. Modifications of the birdcage, such as the use of an RF reflector or “endcap” [53], and modified shapes such as the elliptical [55], or “dome” [56], [57] coils, have been developed. Smaller volume surface coils [58] have been shown to improve image quality, particularly when combined into phased arrays [59]-[67] such as the one shown in Fig. 7. Phased array coils are closer to the area of interest so pick up larger signal strength and are smaller so pick up less noise, thus having higher signal to noise ratio (SNR). Adjacent elements are overlapped so that the mutual inductance between coils is zero. The coupling between non-adjacent elements is greatly decreased using, very low input impedance preamplifiers. Coil to coil interactions are minimized for optimal SNR [59]. Part of the price for this improved image quality is the complexity of the receiver and data acquisition system, as each antenna element requires a separate receiver channel. The image processing is also more computationally expensive, as the signal from each antenna is weighted depending on its proximity to the target region (and hence expected relative SNR), phase shifted, and combined with the other similarly processed signals. Among the practical considerations that are challenging with phased array coils are the expense of additional receiver channels (or the limited number of channels on existing scanners), data acquisition time and the limited field of view, particularly for applications where the region of interest (an arterial occlusion, for instance) may not be precisely known and is therefore easy to miss. Phased-array coils have been used for numerous magnetic resonance angiography (MRA) applications including peripheral [68], [69] abdominal, intracranial and carotid imaging [70] - [72].

Recent coil designs have started to integrate phased-array elements into volume-like coils with the ability to control how the image is constructed to achieve maximum image quality [73], [74]. For these applications, the coil array functions much like the phased array in a synthetic aperture radar application. The image quality for the different coil types and configurations depends strongly on the application. The optimal image construction algorithm depends strongly on the application and region of interest, making the flexibility of being able to synthetically develop large or small subarrays very attractive.

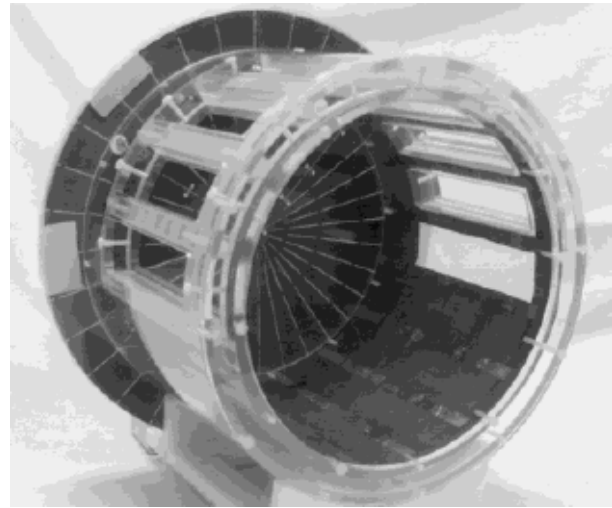


Fig. 6. Quadrature birdcage coil with endcap used for whole-volume head imaging. (Reprinted with permission from [53])

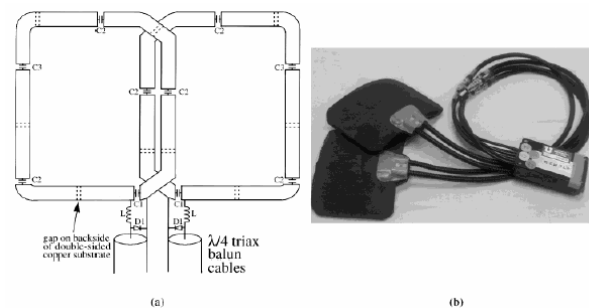


Fig. 7. (a) Two element phased-array coil design. Dashed lines indicate the breaks in the underside of the double-sided copper section of the coil. (b) Image of finished phased array coils (enclosed in foam) with triax balun cables and phased-array port connector box. (Reprinted with permission from [53])

III. ANTENNA ARRAYS FOR HYPERTHERMIA CANCER TREATMENT

Hyperthermia (HT) [78], [79] is a method of treating cancer by heating the body. The tissue is typically heated to 41-45°C for 30-60 min. Often, this involves focusing the energy on the tumor region, relying on the tumor to be more sensitive to heat than the surrounding healthy tissues. HT has also been shown to increase the effectiveness of radiation or chemotherapy [80] - [81]. The most commonly used frequencies for hyperthermia are 433, 915, and 2450 MHz. The type of antenna or antenna array used for HT depends on if it is to be administered superficially, interstitially, or deep-body.

Superficial HT applicators include microstrip [82], waveguide [83], current sheets [84], and the dual concentric conductor antenna, or DCC shown in Fig. 8 [85] -[87]. The DCC is particularly attractive, because it can be easily fabricated on flexible printed circuit board material, which makes it easy to conform to virtually any part of the human body. The DCC aperture is a ring-slot configuration fed simultaneously on all four sides. Prediction and optimization of the heating is normally done by analyzing the near fields of the antenna (the heating region) with numerical methods [86].

Interstitial applicators for HT are typically monopole antennas made from coaxial cables with the center conductor extending beyond the outer ground shield of the cable [88]. These antennas have a tear-drop shaped radiation pattern, so the majority of the heating is near the feedpoint of the antenna (where the ground shield stops), leaving the tip of the antenna extended beyond the useable heating range. The heating distribution can be made more uniform by varying the width of the conductor [89], [90] or adding a choke to the antenna [91]. The heating pattern can be adjusted within the array by phasing the antenna elements [89], [90] or by using nonuniform insulation [92]. Several interstitial applicators were simulated in [93].

Deep body HT applicators are generally based on annular phased arrays (APA) of waveguides [79], coaxial TEM apertures [94], printed antennas [88],[95] and induction systems[96]. Originally, APA systems contained only one ring of 2-D applicators surrounding the patient [97]. The ring could be scanned vertically. Significant improvement with a true 3-D HT system with the applicators vertically offset has been observed [88]. The first clinically used 3-D-type applicator is the SIGMA-Eye applicator (BSD Medical Corp., SLC, UT [98]). A detailed description of this applicator and

different numerical antenna feed models can be found in [98],[99].

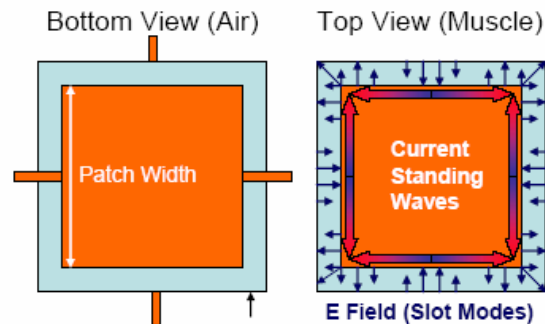


Fig. 8. DCC antenna geometry, E fields in the ring slot and edge currents. (From [85] © 2003 IEEE)

Among the ongoing antenna design challenges in this area is the design of antennas that can be used to also monitor temperature and administer radiation therapy [87], [95], [100]. One prototype combination device is shown in Fig. 9 and another in Fig. 10. Another research area is the use of optimization approaches to predict and control the heating pattern [101], [102]

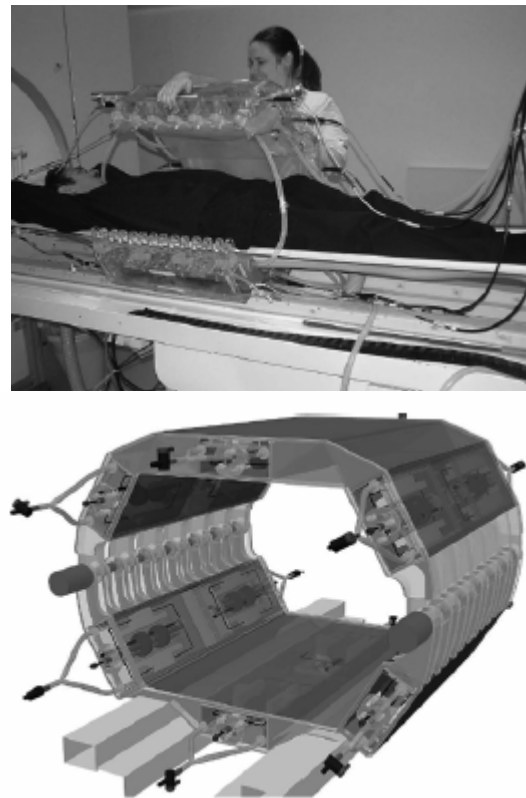


Fig. 9. A prototype of the new Berlin MR-compatible Water-Coated Antenna Applicator (WACOA). (From [100] © 2005 IEEE)

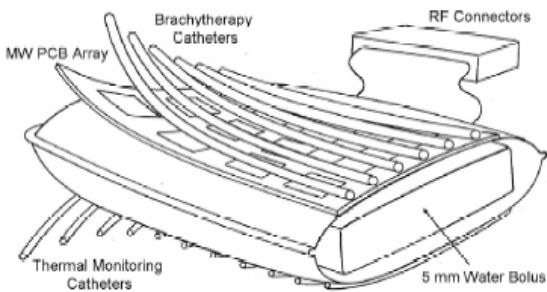


Fig. 10. Schematic of combination applicator showing component parts: parallel catheter arrays for brachytherapy sources and thermal mapping sensors, PCB antenna array, and water coupling bolus. (From [95] © 2004 IEEE)

IV. NUMERICAL SIMULATION METHODS FOR BIOMEDICAL ARRAYS

Several methods for analyzing antenna arrays for medical applications exist. For simple cases where the biological structure can be approximated as uniform or by very simple models such as layers or cylinders, classical methods such as analytical analysis [53], [103] or method of moments [104]-[105] can be used. If the structure of the body varies so much that anatomically-precise modeling is rendered imprecise by variation between individuals, these simple analyses can be used to determine an optimal array design for the range of expected variation between individuals. An example of this was done in [106] for design of coils for vascular MRI. Another example when the body can be modeled as near-uniform is in the case of arrays for hyperthermia of the brain. In [89] stepped-impedance dipoles were modeled using method of moments in an homogenous brain with a localized (non-homogenous) tumor. Method of moments with a simple pulsed basis function (which is the most numerically efficient form) has limitations for heterogeneous models, however, due to artificial charge build up on the dielectric interfaces. [107] Higher order basis functions can overcome this limitation, although the computational complexity is significantly increased [108] - [109]. In addition, the method of moments is very computationally expensive when heterogeneous models are evaluated. It requires $N \log N$ computations, where N is the number of cells in the model, including those making up the heterogeneous object.

A more efficient method for calculation of heterogeneous objects is the finite difference time domain (FDTD) method, which has led to its tremendous popularity for numerical bioelectromagnetic calculations. For example, the interstitial array of

hyperthermia applicators simulated using method of moments in [89] was simulated with a fraction of the computational resources using FDTD in [90]. Several individual hyperthermia applicators have been simulated using FDTD in [93]. FDTD requires N^2 computations, where N is a cell in the (normally cubical) FDTD grid. Unlike method of moments, every cell in space (including at least a minimal amount of air surrounding the model) must be included in the discrete model, so the total number of cells, N , is likely to be larger. However the significant improvement in computational efficiency generally makes this tradeoff favor FDTD for bioelectromagnetic simulations. Complete detailed analysis of breast cancer imaging modalities was also done with FDTD [2]-[25], as well as hyperthermia systems [97], and evaluation of cell phones (including those with dual antennas) near the human head. [110],[111] Antennas for implantation in the body (mostly microstrip or PIFA types) have been simulated with FDTD and in some cases optimized with genetic algorithms [112]. Deep hyperthermia applicators (annular phased arrays) have been simulated extensively with FDTD [113]-[115].

Several FDTD developments have been important for bioelectromagnetic simulations including the development of frequency-dependent methods (FD)²TD, [116] low frequency FDTD methods, [117] efficient FDTD computation, [118] and evaluation of temperature using the bioheat equation [115].

Model development is one of the significant challenges of numerical bioelectromagnetics. Models have progressed from the prolate spheroidal models of the human used during the 1970s [119] to roughly 1cm models based on anatomical cross sections used during the 1980s [120] to a new class of millimeter-resolution MRI-based models of the body that have been the hallmarks of research since the 1990s [121]-[124]. Today probably the most widely used models are derived from the Visible Man Project [125].

Once a tissue-segmented model has been chosen, the electrical properties of the tissues are defined. The properties of human tissue change significantly with frequency, so it is essential to use data accurately measured at the frequency of interest. There is a wide range of published data on measured tissue properties [28] -[35], [119], [126]-[129], and work is still underway to measure and verify these properties. These and other references are electronically searchable at [130].

Periodic boundary conditions are available for method of moments [131], [132] and the FDTD method [133] - [138] for predicting array behavior from

evaluation of a single antenna in the array. These may have application in antenna arrays for medical applications; however they have not been used in this application space yet. This is no doubt due at least in part to the fact that the nearby human body is neither uniform nor periodic in shape.

VI. CONCLUSIONS

The applications for phased arrays in medicine have borrowed strongly from other applications of phased arrays, particularly those seen in radar. Imaging methods including tomography, confocal imaging, thermography, and MRI provide enhanced medical imaging. Hyperthermia treatments often improve the outcome of radiation and chemotherapy for cancer treatment. A wide variety of antennas have been used in these arrays, and the arrays have been produced either physically or synthetically by scanning a single antenna or pair of antennas over the region of interest. The arrays have been phased either electronically, or (more commonly) by time delaying the received signals during recombination. Design challenges for these applications include making the antennas small enough to be physically useable, coupling the signal to the body with minimal reflection, using low enough frequency to penetrate lossy biological material yet high enough frequency to obtain good resolution. Among the current research challenges are optimized design of the arrays for a variety of configurations and integration of other technologies (radiation therapy and temperature monitoring, for instance) with the antenna design. Applications for phased array antennas promise continued growth in the medical arena.

ACKNOWLEDGEMENTS

The author gratefully acknowledges the assistance of Dr. Rock Hadley for contributions to the MRI section of this paper.

REFERENCES

- [1] D. Colton and P. Monk, "A new approach to detecting leukemia: Using computational electromagnetics," *IEEE Trans. Comput. Sci. Eng.*, vol.2, pp. 46–52, winter 1995.
- [2] P. M. Meaney, M. W. Fanning, D. Li, S. P. Poplack, and K. D. Paulsen, "A clinical prototype for active microwave imaging of the breast," *IEEE Trans. Microwave Theory Tech.*, vol. 48, pp. 1841-1853, Nov. 2000.
- [3] W. C. Chew and J. H. Lin, "A frequency-hopping approach for microwave imaging of large inhomogeneous bodies," *IEEE Microwave Guided Wave Lett.*, vol. 5, pp. 439–441, Dec. 1995.
- [4] O. S. Haddadin and E. S. Ebbini, "Imaging strongly scattering media using a multiple frequency distorted Born iterative method," *IEEE Trans. Ultrason., Ferroelect., Freq. Contr.*, vol. 45, pp. 1485–1496, Nov. 1998.
- [5] Q. Fang, P. M. Meaney, and K. D. Paulsen, "Microwave image reconstruction of tissue property dispersion characteristics utilizing multiple-frequency information," *IEEE Trans. Microwave Theory Tech.*, vol. 52, pp. 1866-1875, Aug. 2004.
- [6] P. M. Meaney, K. D. Paulsen, A. Hartov, and R. C. Crane, "An active microwave imaging system for reconstruction of 2-D electrical property distributions," *IEEE Trans. Biomed. Imag.*, vol. 42, pp. 1017–1026, Oct. 1995.
- [7] K. D. Paulsen and P. M. Meaney, "Compensation for nonactive array element effects in a microwave imaging system: Part I—Forward solution vs. measured data comparison," *IEEE Trans. Med. Imag.*, vol. 18, pp. 496–507, June 1999.
- [8] P. M. Meaney, K. D. Paulsen, M. W. Fanning, and A. Hartov, "Nonactive antenna compensation for fixed-array microwave imaging: Part II—Imaging results," *IEEE Trans. Med. Imag.*, vol. 18, pp. 508-518, Jun. 1999.
- [9] P. M. Meaney, K. D. Paulsen, A. Hartov, and R. K. Crane, "Microwave imaging for tissue assessment: Initial evaluation in multitarget tissue-equivalent phantoms," *IEEE Trans. Biomed. Eng.*, vol. 43, pp. 878-890, Sept. 1996.
- [10] E. C. Fear, S. C. Hagness, P. M. Meaney, M. Okieniewski, and M. Stuchly, "Enhancing breast cancer detection using near field imaging," *IEEE Microwave Magazine*, pp. 48-56, March 2002.
- [11] S. C. Hagness, A. Taflove, and J. E. Bridges, "Two-dimensional FDTD analysis of a pulsed microwave confocal system for breast cancer detection: Fixed-focus and antenna-array sensors," *IEEE Trans. Biomed. Eng.*, vol. 45, pp. 1470–1479, Dec. 1998.
- [12] S. C. Hagness, A. Taflove, and J. E. Bridges, "Three-dimensional FDTD analysis of a pulsed microwave confocal system for breast cancer detection: Design of an antenna-array element," *IEEE Trans. Antennas Propagat.*, vol. 47, pp. 783–791, May 1999.
- [13] X. Li and S. C. Hagness, "A confocal microwave imaging algorithm for breast cancer detection," *IEEE Microwave Wireless Comp. Lett.*, vol. 11, pp. 130–132, Mar. 2001.
- [14] E. Fear and M. Stuchly, "Microwave system for breast tumor detection," *IEEE Microwave Guided Wave Lett.*, vol. 9, pp. 470–472, Nov. 1999.

- [15] E. C. Fear and M. A. Stuchly, "Microwave detection of breast cancer," *IEEE Trans. Microwave Theory Tech.*, vol. 48, pp. 1854–1863, Nov. 2000.
- [16] X. Yun, E. C. Fear, and R. H. Johnston, "Compact Antenna for Radar-Based Breast Cancer Detection," *IEEE Trans. Antennas and Propagation*, vol. 53, no. 8, pp. 2374–2380, Aug. 2005.
- [17] S. C. Hagness, A. Taflove, and J. E. Bridges, "Wideband ultralow reverberation antenna for biological sensing," *Electronic Lett.*, vol. 33, no. 19, pp. 1594–1595, Sep. 1997.
- [18] M. A. Hernandez-Lopez, M. Pantoja, M. Fernandez, S. Garcia, A. Bretones, R. Martin, and R. Gomez, "Design of an ultra-broadband V antenna for microwave detection of breast tumors," *Microw. Opt. Tech. Lett.*, vol. 34, no. 3, pp. 164–166, Aug. 2002.
- [19] E. C. Fear and M. A. Stuchly, "Microwave breast tumor detection: Antenna design and characterization," *IEEE Antennas Propag. Symp. Dig.*, vol. 2, pp. 1076–1079, 2000.
- [20] X. Li, S. C. Hagness, M. K. Choi, and D. W. W. Choi, "Numerical and experimental investigation of an ultrawideband ridged pyramidal horn antenna with curved launching plane for pulse radiation," *IEEE Antennas Wireless Propag. Lett.*, vol. 2, pp. 259–262, 2003.
- [21] X. Yun, E. C. Fear, and R. H. Johnston, "Radar-based microwave imaging for breast cancer detection: Tumor sensing with cross-polarized reflections," *IEEE Antennas Propag. Society Symp. Dig.*, vol. 3, pp. 2432–2435, 2004.
- [22] C. J. Shannon, E. C. Fear, and M. Okoniewski, "Dielectric-filled slotline bowtie antenna for breast cancer detection," *Electronics Letters*, vol. 41, no. 7, March 2005.
- [23] J. M. Sill and E. C. Fear, "Tissue sensing adaptive radar for breast cancer detection: A study of immersion liquid," *Electronics Letters*, vol. 41, no. 3, pp. 113–115, Feb. 2005.
- [24] J. M. Sill and E. C. Fear, "Tissue sensing adaptive radar for breast cancer detection: Preliminary experimental results," *IEEE MTT-S Int. Microwave Symp. Dig.*, Long Beach, CA, June 2005.
- [25] J. M. Sill and E. C. Fear, "Tissue Sensing Adaptive Radar for Breast Cancer Detection—Experimental Investigation of Simple Tumor Models," *IEEE Trans. Microwave Theory Tech.*, vol. 53, no. 11, pp. 3312–3319, Nov. 2005.
- [26] S. Y. Semenov, A. E. Bulyshev, A. E. Souvorov, R. H. Svenson, Y. E. Sizov, V. Y. Borisov, V. G. Posukh, I. M. Kozlov, A. G. Nazarov, and G. P. Tatsis, "Microwave tomography: Theoretical and experimental investigation of the iteration reconstruction algorithm," *IEEE Trans. Microw. Theory Tech.*, vol. 46, pp. 133–141, Feb. 1998.
- [27] S. Y. Semenov, R. H. Svenson, A. E. Bulyshev, A. E. Souvorov, A. G. Nazarov, Y. E. Sizov, V. G. Posukh, and A. Pavlovsky, "Three-dimensional microwave tomography: Initial experimental imaging of animals," *IEEE Trans. Biomed. Eng.*, vol. 49, pp. 55–63, Jan. 2002.
- [28] C. Gabriel, S. Gabriel, and E. Corthout, "The dielectric properties of biological tissues: I. Literature survey," *Phys. Med. Biol.*, vol. 41, pp. 2231–2249, 1996.
- [29] S. Gabriel, R. W. Lau, and C. Gabriel, "The dielectric properties of biological tissues: II. Measurements on the frequency range 10 Hz to 20 GHz," *Phys. Med. Biol.*, vol. 41, pp. 2251–2269, 1996.
- [30] S. Gabriel, R. W. Lau, and C. Gabriel, "The dielectric properties of biological tissues: III. Parametric models for the dielectric spectrum of tissues," *Phys. Med. Biol.*, vol. 41, pp. 2271–2293, 1996.
- [31] K. R. Foster and H. P. Schwan, "Dielectric properties of tissues and biological materials: A critical review," *Crit. Rev. Biomed. Eng.*, vol. 17, pp. 25–104, 1989.
- [32] S. S. Chaudhary, R. K. Mishra, A. Swarup, and J. M. Thomas, "Dielectric properties of normal and malignant human breast tissues at radiowave and microwave frequencies," *Indian J. Biochem. Biophys.*, vol. 21, pp. 76–79, 1984.
- [33] A. J. Surowiec, S. S. Stuchly, J. R. Barr, and A. Swarup, "Dielectric properties of breast carcinoma and the surrounding tissues," *IEEE Trans. Biomed. Eng.*, vol. 35, pp. 257–263, Apr. 1988.
- [34] W. T. Joines, Y. Z. Dhenxing, and R. L. Jirtle, "The measured electrical properties of normal and malignant human tissues from 50 to 900 MHz," *Med. Phys.*, vol. 21, pp. 547–550, 1994.
- [35] A. M. Campbell and D. V. Land, "Dielectric properties of female human breast tissue measured in vitro at 3.2 GHz," *Phys. Med. Biol.*, vol. 37, pp. 193–210, 1992.
- [36] K. L. Carr, "Microwave radiometry: Its importance to the detection of cancer," *IEEE Trans. Microwave Theory Tech.*, vol. 37, no. 12, pp. 1862–1869, Dec. 1989.
- [37] K. L. Carr, "Radiometric sensing," *IEEE Potentials*, pp. 21–25, April/May 1997.
- [38] L. Dubois, J. – P. Sozanski, V. Tessier, J. –C. Camart, J. –J. Fabre, J. Pribetich, and M. Chiv, "Temperature Control and Thermal Dosimetry by Microwave Radiometry in Hyperthermia," *IEEE*

- Trans. Microwave Theory Tech.*, vol. 44, no. 10, pp. 1755-1761, Oct. 1996.
- [39] S. M. Fraser, D. V. Land, and R. D. Sturrock, "Microwave Thermography - an Index of Inflammatory Disease," *Br. J. Rheumatology*, vol. 26, pp. 37-39, 1987.
- [40] B. Bocquet, J. C. Van de Velde, A. Mamouni, and Y. Leroy, "Microwave radiometric imaging at 3 GHz for the exploration of breast tumours," *IEEE Trans. Microwave Theory Tech.*, vol. 38, pp. 791-793, 1990.
- [41] J. Robert, J. Edrich, P. Thouvenot, M. Gautherie, and J. M. Escanye, "Millimeter wave thermography: Preliminary clinical finding on head and neck diseases," *J. Microwave Power*, vol. 14, 1979.
- [42] K. L. Carr, A. M. ElMahdi, and J. Schaeffer, "Dual mode microwave system to enhance early detection of cancer," *IEEE Trans. Microwave Theory Tech.*, vol. 29, pp. 256-260, 1980.
- [43] E. A. Cheever, J. B. Leonard, and K. R. Foster, "Depth of penetration of fields from rectangular apertures into lossy media," *IEEE Trans. Microwave Theory Tech.*, vol. 35, pp. 865-867, 1987.
- [44] J. Audet, J. C. Bolomey, C. Pichot, D. D. n'Guyen, M. Robillard, M. Chive, and Y. Leroy, "Electrical characteristics of waveguide applicators for medical applications," *J. Microwave Power*, vol. 15, pp. 177-186, 1980.
- [45] A. W. Guy, "Electromagnetic fields and relative heating patterns due to a rectangular aperture source in direct contact with bilayered biological tissue," *IEEE Trans. Microwave Theory Tech.*, vol. 29, pp. 214-223, 1971.
- [46] D. V. Land, "Medical microwave radiometry and its clinical applications," *IEE Colloquium Application of Microwaves in Medicine*, pp. 2/1 - 2/5, 28 Feb 1995.
- [47] B. Enander and G. Larson, "Microwave radiometry measurements of the temperature inside a body," *Electronic Letters*, vol. 10, pp. 317, 1974.
- [48] J. Edrich and P. C. Hardee, "Thermography at millimeter wavelengths," *Proc. IEEE*, vol. 62, pp. 1391-1392, 1974.
- [49] E. A. Cheever and K. R. Foster, "Microwave radiometry in living tissue: What does it measure?" *IEEE Trans. Biomedical Engineering*, vol. 39, no. 6, pp. 563-568, June 1992.
- [50] B. Bocquet, J. C. van de Velde, A. Mamouni, Y. Leroy, G. Giauz, J. Delannoy, and D. Delvallee, "Microwave Radiometric Imaging at 3 GHz for the Exploration of Breast Tumors," *IEEE Trans. Microwave Theory Tech.*, vol. 38, no.6, pp. 791-793, June 1990.
- [51] L. Enel, Y. Leroy, J. C. Van de Velde, and A. Mamouni, "Improved recognition of thermal structures by microwave radiometry," *Electronics Letters*, vol. 20, pp. 293-294, 1984.
- [52] Y. Leroy, A. Mamouni, J. C. Van de Velde, B. Bocquet, and B. Dujardin, "Microwave radiometry for non invasive thermometry," *Automedica (Special Issue on Noninvasive Thermometry)*, vol. 8, pp. 181-201, 1987.
- [53] J. R. Hadley, B. E. Chapman, J. A. Roberts, D. C. Chapman, K. C. Goodrich, H. R. Buswell, A. L. Alexander, J. S. Tsuruda, and D. L. Parker, "A Three-Coil Comparison for MR Angiography," *Journal of Magnetic Resonance Imaging*, 11 pp. 458-468, 2000.
- [54] C. E. Hayes, W. A. Edelstein, and J. F. Schenck, et al., "An efficient, highly homogeneous radiofrequency coil for whole-body NMR imaging at 1.5 T," *J. Magn. Reson. Imaging*, vol. 63, pp. 622-628, 1985.
- [55] M. C. Leifer, "Theory of the quadrature elliptic birdcage coil," *Magn. Reson. Med.*, vol. 38 pp. 726-732, 1997.
- [56] S. Li, C. M. Collins, and B. J. Dardzinski, et al., "A method to create an optimum current distribution and homogeneous B1 field for elliptical birdcage coils," *Magn. Reson. Med.*, vol. 37, pp. 600-608, 1997.
- [57] J. R. Fitzsimmons, J. C. Scott, and D. M. Peterson, et al., "Integrated RF coil with stabilization for FMRI human cortex," *Magn. Reson. Med.*, vol. 38, pp. 15-18, 1997.
- [58] L. E. Hendrix, J. A. Strandt, and D. L. Daniels, et al., "Three-dimensional time-of-flight MR angiography with a surface coil: evaluation in 12 subjects," *American Journal Radiology*, vol. 159, pp. 103-106, 1992.
- [59] P. B. Roemer, W. A. Edelstein, C. E. Hayes, S.P.Souza, and O.M.Mueller, "The NMR phased array," *Magn. Reson. Med.*, 16(2), pp. 192-225, 1996.
- [60] C. E. Hayes, N. Hattes, and P. B. Roemer, "Volume imaging with MR phased arrays," *Magn. Reson. Med.*, vol. 18, no. 2, pp. 309-319, 1991.
- [61] C. E. Hayes and P. B. Roemer, "Noise correlations in data simultaneously acquired from multiple surface coil arrays," *Magn. Reson. Med.*, vol. 16, no. 2, pp. 181-191, 1991.
- [62] S. M. Wright, R. L. Magin, and J. R. Kelton, "Arrays of mutually coupled receiver coils: theory and application," *Magn. Reson. Med.*, vol. 17, no. 1, pp. 252-268, 1991.
- [63] S. M. Wright and L. L. Wald, "Theory and application of array coils in MR spectroscopy," *NMR Biomed.*, vol. 10, no. 8, pp. 394-410, 1997.

- [64] G. R. Duensing, H. R. Brooker, and J. R. Fitzsimmons, "Maximizing signal-to-noise ratio in the presence of coil coupling," *Magn. Reson. B*, vol. 111, no. 3, pp. 230-235, 1996.
- [65] D. K. Sodickson and W. J. Manning, "Simultaneous acquisition of spatial harmonics (SMASH): ultra-fast imaging with radiofrequency coil arrays," *Magn. Reson. Med.*, vol. 38, pp. 591-603, 1997.
- [66] K. P. Pruessmann, M. Weiger, M. B. Scheidegger, and P. Boesiger, "SENSE: Sensitivity encoding for fast MRI," *Magn. Reson. Med.*, vol. 42, pp. 952-962, 1999.
- [67] Y. Zhu, "Parallel excitation with an array of transmit coils," *Magn. Reson. Med.*, vol. 51, no. 4, pp. 775-784, 2004.
- [68] K. Y. Kojima, J. Szumowski, and R. C. Sheley, et al., "Lower extremities: MRangiography with a unilateral telescopic phased-array coil," *Radiology*, 196, pp. 871-875, 1995.
- [69] J. W. Monroe, P. Schmalbrock, and D. G. Spigos, "Phased array coils for upper extremity MRA," *Magn. Reson. Med.*, vol. 33, pp. 224-229, 1995.
- [70] C. E. Hayes, C. M. Mathis, and C. Yuan, "Surface coil phased arrays for high-resolution imaging of the carotid arteries," *Magn. Reson. Imaging*, vol. 1, pp. 109-112, 1996.
- [71] C. Yuan, J. W. Murakami, and C. E. Hayes, et al, "Phased-array magnetic resonance imaging of the carotid artery bifurcation: preliminary results in healthy volunteers and a patient with atherosclerotic disease," *Magn. Reson. Imaging*, vol. 5, pp. 561-565 1995.
- [72] S. H. Faro, S. Vinitiski, and H. V. Ortega, et al, "Carotid magnetic resonance angiography: improved image quality with dual 3-inch surface coils," *Neuroradiology*, vol. 38, pp. 403-408, 1996.
- [73] H. A. Stark and E. M. Haacke, "Helmet and cylindrical shaped CP array coils for brain imaging: a comparison of signal-to-noise characteristics," *Proceedings of the International Society for Magnetic Resonance in Medicine*, pp. 1412, 1996.
- [74] J. R. Porter, S. M. Wright, and A. Reykowski, "A 16-element phased-array head coil," *Magn. Reson. Med.*, vol. 40, pp. 272-279, 1998.
- [75] T. Wu and R. King, "The cylindrical antenna with nonreflecting resistive loading," *IEEE Trans. Antennas Propag.*, vol. AP-13, no. 3, pp. 369-373, May 1965.
- [76] T. Wu and R. King, "Corrections to 'The cylindrical antenna with nonreflecting resistive loading'," *IEEE Trans. Antennas Propag.*, vol. AP-13, no. 11, p.998, Nov. 1965.
- [77] E. C. Fear, J. Sill, and M. A. Stuchly, "Experimental Feasibility Study of Confocal Microwave Imaging for Breast Tumor Detection," *IEEE Trans. Microwave Theory Tech.*, vol. 51, no. 3, pp. 887-892, March 2003.
- [78] *Special Issue of IEEE Trans. Microwave Theory Tech.*, MTT-34, 1986.
- [79] C. H. Durney and M. F. Iskander, *Antenna Handbook*. Eds. Y.T. Lo & S.W. Lee, 1993.
- [80] P. K. Sneed and T. L. Phillips, "Combining hyperthermia and radiation: How beneficial?," *Oncology*, vol. 5, pp. 99-108, 1991.
- [81] C. C. Vernon, J. W. Hand, and S. B. Field, et al., "Radiotherapy with or without hyperthermia in the treatment of superficial localized breast cancer: Results from five randomized controlled trials," *Int. J. Radiat. Oncol. Biol. Phys.*, vol. 35, pp. 731-44, 1996.
- [82] F. Montecchia, "Microstrip antenna design for hyperthermia treatment of superficial tumors," *IEEE Trans. BME*, vol. 39, no. 6, pp. 580-588, June 1992,
- [83] J. Vba, C. Franconi, F. Montecchia, and I. Vannucci, "Evanescent-Mode Applicators (EMA) for superficial and subcutaneous hyperthermia," *IEEE Trans. Biomed. Eng.*, vol. 40, no.5, pp. 397-407, May 1993.
- [84] M. V. Prior, M. L. D. Lumori, J. W. H. G. Lamaitre, C. J. Schneider, and J. D. P. van Dijk, "The Use of a Current Sheet Applicator Array for Superficial Hyperthermia: Incoherent Versus Coherent Operation," *IEEE Trans. Biomed. Eng.*, vol. 43, no. 7, pp. 694-698, July 1995.
- [85] P. R. Stauffer, M. Leoncini, and V. Manfrini, et al., "Dual concentric conductor radiator for microwave hyperthermia with improved field uniformity to periphery of aperture," *IEICE Trans. on Communicat.*, vol. E78-B, pp. 826-35, 1995.
- [86] P. F. Maccarini, H. Rolfsnes, D. Neuman and P. Stauffer, "Optimization of a Dual Concentric Conductor Antenna for Superficial Hyperthermia Applications," *Proceedings of the 26th Annual International conference of the IEEE EMBS*, San Francisco, CA, USA, September 1-5, 2004.
- [87] S. Jacobsen, P. R. Stauffer, and D. G. Neuman, "Dual-mode antenna design for microwave heating and noninvasive thermometry of superficial tissue disease," *IEEE Trans. Biomed. Eng.*, vol. 47, 2000.
- [88] P. F. Turner, "Interstitial Equal-Phased Arrays for EM Hyperthermia," *IEEE Trans. Microwave Theory and Tech.*, vol. 34, no.5, pp. 572 - 578, May 1986.
- [89] C. M. Furse and M. F. Iskander, "Three-dimensional Electromagnetic Power Deposition in Tumors using Interstitial Antenna Arrays,"

- IEEE Trans. on Biomedical Engineering*, vol. 36, pp. 977-986, Oct. 1989.
- [90] P. Cherry and M. F. Iskander, "FDTD analysis of power deposition patterns of an array of interstitial antennas for use in microwave hyperthermia," *IEEE Trans. Microwave Theory and Tech.*, vol. 40, no. 8, pp. 1692-1700, Aug 1992.
- [91] R. D. Nevels, G. D. Arndt, G. W. Raffoul, J. R. Carl, and A. Pacifico, "Microwave catheter design," *IEEE Trans. on Biomedical Engineering*, vol. 45, pp.885-890, July 1998.
- [92] C. Manry, S. L. Broschat, C.-K. Chou, and J. A. McDougall, "An eccentrically coated asymmetric antenna applicator for intracavity hyperthermia treatment of cancer," *IEEE Trans. on Biomedical Engineering*, vol. 39, no. 9, pp. 935-942, Sept. 1992.
- [93] J. C. Camart, D. Despretz, M. Chive, and J. Pribetich, "Modeling of various kinds of applicators used for microwave hyperthermia based on the FDTD method," *IEEE Trans. Microwave Theory and Tech.*, vol. 44, no. 10, pp. 1811-1818, Oct. 1996.
- [94] P. F. Turner, "Hyperthermia and Inhomogeneous Tissue Effects Using an Annular Phased Array," *IEEE Trans. Microwave Theory and Tech.*, vol. 32, no. 8, pp. 874 - 875, Aug. 1984.
- [95] P. Stauffer, J. Schlorff, R. Taschereau, T. Juang, D. Neuman, P. Maccarini, J. Pouliot and J. Hsu, "Combination Applicator for Simultaneous Heat and Radiation," *Proceedings of the 26th Annual International Conference of the IEEE EMBS*, San Francisco, CA, September 1-5, 2004.
- [96] Y. Kotsuka, E. Hankui, and Y. Shigematsu, "Development of Ferrite Core Applicator System for Deep-Induction Hyperthermia," *IEEE Trans. Microwave Theory and Tech.*, vol. 44, no. 10, pp. 1803-1810, Oct. 1996.
- [97] D. M. Sullivan, "Three-dimensional computer simulation in deep regional hyperthermia using the FDTD Method," *IEEE Trans. Microwave Theory and Tech.*, vol. 38, no. 2, pp. 201-211, Feb. 1990.
- [98] P. F. Turner, "Sigma 60-24 Prototype Test Results," *BSD Medical Corporation*, Salt Lake City, UT, Internal Rep., 1992.
- [99] J. Nadobny, H. Föhling, M. Hagmann, P. Turner, W. Wlodarczyk, J.Gellermann, P. Deuflhard, and P. Wust, "Experimental and numerical investigations of feed-point parameters in a 3-D hyperthermia applicator using different models of feed networks," *IEEE Trans. Biomed. Eng.*, vol. 49, no. 11, pp. 1348-1359, Nov. 2002.
- [100] J. Nadobny, W. Wlodarczyk, L. Westhoff, J. Gellermann, R. Felix, and P. Wust, "A Clinical Water-Coated Antenna Applicator for MR-Controlled Deep-Body Hyperthermia: A Comparison of Calculated and Measured 3-D Temperature Data Sets," *IEEE Trans. on Biomedical Engineering*, vol. 52, no. 3, pp. 505-519, March 2005.
- [101] K. S. Nikita and N. K. Uzunoglu, "Coupling Phenomena in Concentric Multi-Applicator Phased Array Hyperthermia Systems," *IEEE Trans. Microwave Theory and Tech.*, vol. 44, no. 1, pp. 65-74, Jan 1996.
- [102] F. Bardati, A. Borrani, A. Gerardino, and G. A. Lovisolo, "SAR Optimization in a Phased Array Radiofrequency Hyperthermia System," *IEEE Trans. on Biomedical Engineering*, vol. 42, no. 12, pp. 1201-1207, Dec. 1995.
- [103] R. W. P. King, G. J. Fikioris, and R. B. Mack, *Cylindrical Antennas and Arrays*, Cambridge, U.K.: Cambridge Univ. Press, 2002.
- [104] S. Ebihara and T. Yamamoto, "Resonance analysis of a circular dipole array antenna in cylindrically layered media for directional borehole radar," *IEEE Trans. Geosci. Remote Sensing*, vol. 44, no.1, pp. 22-31, Jan. 2006.
- [105] K. Holliger and T. Bergmann, "Numerical modeling of borehole geo-radar data," *Geophysics*, vol. 67, no. 4, pp. 1249-1257, July/Aug. 2002.
- [106] J. R. Hadley, "Design of Radio Frequency Coil Arrays for Optimal Signal to Noise Ratio for Magnetic Resonance Angiography," PhD Dissertation, University of Utah Electrical and Computer Engineering Department, 2005.
- [107] H. Massoudi, C. H. Durney, and M. F. Iskander, "Limitations of the cubical block model of man in calculating SAR distribution," *IEEE Trans. Microwave Theory and Tech.*, vol. 32, pp. 746-752, 1984.
- [108] C. T. Tsai, H. Massoudi, C. H. Durney, and M. F. Iskander, "A procedure for calculating fields inside arbitrarily-shaped, inhomogeneous dielectric bodies using linear basis functions with the moment method," *IEEE Trans. Microwave Theory and Tech.*, vol. 34, pp. 1131-1139, 1986.
- [109] O. H. Schaubert, D. R. Wilton, and A. W. Glisson, "A tetrahedral modeling method of electromagnetic scattering by arbitrarily shaped inhomogeneous objects," *IEEE. Trans. Antennas and Propagation*, vol. 32, pp. 75-82, 1984.
- [110] B. M. Green and M. A. Jensen, "Diversity performance of dual-antenna handsets near operator tissue," *IEEE. Trans. Antennas and Propagation*, vol. 48, no. 7, pp. 1017-1024, July 2000.
- [111] O. Gandhi, G. Lazzi, and C. Furse, "Electromagnetic Absorption in the Human Head

- and Neck for Mobile Telephones at 835 and 1900 MHz," *IEEE Trans. on Microwave Theory and Tech.*, vol. 44, pp. 1884-1897, 1996.
- [112] P. Soontornpipit, C. M. Furse, and Y. C. Chung, "Design of Implantable Microstrip Antenna for Communication with Medical Implants," *Special Issue of IEEE Trans. on Microwave Theory and Tech. on Medical Applications and Biological Effects of RF/Microwaves*, Sept. 2004.
- [113] C. E. Reuter, A. Taflove, V. Sathiseelan, M. Piket-May, and B. B. Mittral, "Unexpected physical phenomena indicated by FDTD modeling of the Sigma-60 deep hyperthermia applicator," *IEEE Trans. Microwave Theory and Tech.*, vol. 46, no.4, pp. 313-319, April 1998.
- [114] C.-Q. Wang and O. P. Gandhi, "Numerical simulation of annular phased arrays for anatomically based models using the FDTD method," *IEEE Trans. Microwave Theory and Tech.*, vol. 37, no.1, pp. 118-126, Jan, 1989.
- [115] D. Sullivan, D. Buechler, and F. A. Gibbs, "Comparison of measured and simulated data in an annular phased array using an inhomogeneous phantom," *IEEE Trans. Microwave Theory and Tech.*, vol. 40, no.3, pp. 600-604, Mar. 1992.
- [116] C. M. Furse, J.-Y. Chen, and O. P. Gandhi, "Use of the Frequency-Dependent Finite-Difference Time-Domain Method for Induced Current and SAR Calculations for a Heterogeneous Model of the Human Body," *IEEE Trans. on Electromagnetic Compatibility*, pp.128-133, May 1994.
- [117] C. Furse and O. P. Gandhi, "Calculation of Electric Fields and Currents Induced in a Millimeter-Resolution Human Model at 60 Hz Using the FDTD Method," *Bioelectromagnetics*, 19 (5), pp.293-299, 1998.
- [118] C. M. Furse and O. P. Gandhi, "A Memory Efficient Method of Computing Specific Absorption Rate in CW FDTD Simulations," *IEEE Transactions on Biomedical Engineering*, vol. 43, no. 5, pp. 558-560, May 1996.
- [119] C. H. Durney, C. C. Johnson, P. W. Barber, H. Massoudi, M. F. Iskander, J. L. Lords, D. K. Ryser, S. J. Allen, and J. C. Mitchell, *Radiofrequency Radiation Dosimetry Handbook*, 2nd ed., USAF School of Medicine, Brooks AFB, TX, 1978.
- [120] O. P. Gandhi, Y. G. Gu, J. Y. Chen, and H. I. Bassen, "Specific absorption rates and induced current distributions in an anatomically based human model for plane-wave exposures," *Health Physics*, 63(3), pp. 281-290, 1992.
- [121] O. P. Gandhi and C. M. Furse, "Millimeter-resolution MRI-based models of the human body for electromagnetic dosimetry from ELF to microwave frequencies," *Voxel Phantom Development: Proceedings of an International Workshop held at the National Radiological Protection Board*, Chilton, UK, July 6-7, 1995, Peter J. Dimbylow, editor.
- [122] P. J. Dimbylow, "The development of realistic voxel phantoms for electromagnetic field dosimetry," *Voxel Phantom Development: Proceedings of an International Workshop held at the National Radiological Protection Board*, Chilton, UK, July 6-7, 1995, Peter J. Dimbylow, editor.
- [123] P. Olley and P. S. Excell, "Classification of high resolution voxel image of a human head," *Voxel Phantom Development: Proceedings of an International Workshop held at the National Radiological Protection Board*, Chilton, UK, July 6-7, 1995, Peter J. Dimbylow, editor.
- [124] M. A. Stuchly, K. Caputa, A. van Wensen, and A. El-Sayed, "Models of human and animal bodies in electromagnetics," *Voxel Phantom Development: Proceedings of an International Workshop held at the National Radiological Protection Board*, Chilton, UK, July 6-7, 1995, Peter J. Dimbylow, editor.
- [125] National Library of Medicine, Visible Man Project, MRI scans, CT scans, and photographs available on CD through Research Systems, Inc., 2995 Wilderness Place, Boulder, CO 80301.
- [126] C. Gabriel, "Compilation of the dielectric properties of body tissues at RF and microwave frequencies," *Final Report AL/OE-TR-1996-0037 submitted to Occupational and Environmental Health Directorate, RFR Division*, 2503 Gillingham Dr., Brooks AFB, TX, June 1996.
- [127] M. A. Stuchly and S. S. Stuchly, "Dielectric properties of biological substances – tabulated," *J. Microwave Power*, 15 (1), pp. 19-26, 1980.
- [128] S. Rush, J. A. Abildskov, and R. McFee, "Resistivity of body tissues at low frequencies," *Circ. Research*, vol. XII, pp. 40-50, 1963.
- [129] L. A. Geddes and L. E. Baker, "The specific resistance of biological material – a compendium of data for the biomedical engineer and physiologist," *Med. & Biol. Engng.*, vol. 5, pp. 271-293, Pergamon Press., 1967.
- [130] University of Utah Dielectric Database OnLine <http://www.ece.utah.edu/dielectric/>
- [131] D. M. Pozar, "Microstrip antennas," *Proc. IEEE*, vol. 80, pp. 79-91, Jan 1992.
- [132] A. Cucini, M. Albani, and S. Maci, "Truncated floquet wave full-wave analysis of large phased arrays of open-ended waveguides with nonuniform amplitude excitation," *IEEE Trans. Antennas and Propagation*, vol. 51, no.6, pp. 1386-1394, June 2003.

- [133] G. Turner and C. Christodoulou, "FDTD analysis of phased array antennas," *IEEE Trans. Antennas and Propagation*, vol. 47, no. 4, pp. 661-667, April 1999.
- [134] J. Ren, O. P. Gandhi, L. R. Walker, J. Frascilla, and C. R. Boerman, "Floquet-based FDTD analysis of two-dimensional phased array antennas," *IEEE Microwave and Guided Wave Letters*, vol. 4, no.4, pp. 109-111, April 1994.
- [135] C. Railton and G. S. Hilton, "The analysis of medium-sized arrays of complex elements using a combination of FDTD and reaction matching," *IEEE Trans. Antennas and Propagation*, vol. 47, no. 4, pp. 707-714, April 1999.
- [136] J. Gomez-Tagle, P. Wahid, M. Chryssomallis, and C. Christodoulou, "FDTD analysis of finite-sized phased array microstrip antennas," *IEEE Trans. Antennas and Propagation*, vol. 51, no. 8, pp. 2057-2062, Aug. 2003.
- [137] H. Holter and H. Steyskal, "On the size requirement for finite phased-array models," *IEEE Trans. Antennas and Propagation*, vol. 50, no. 6, pp. 836-840, June 2002.
- [138] T. Su, N.-T. Huang, Y. Lio, W. Yu, and R. Mittra, "Investigation of instability characteristics arising in the FDTD simulation of electrically large antenna arrays," *IEEE Antennas and Propagation Society International Symposium*, vol. 1, pp. 1014-1017, June 2004.



Dr. Cynthia Furse is the Director of the Center of Excellence for Smart Sensors at the University of Utah and Professor in the Electrical and Computer Engineering Department. The Center focuses on imbedded antennas and sensors in complex environments, such as telemetry systems in the human body, and sensors for location of faults on aging aircraft wiring. Dr. Furse has directed the Utah "Smart Wiring" program, sponsored by NAVAIR and USAF, since 1998. She is Head of Research for LiveWire Test Labs, Inc., a spin off company commercializing devices to locate intermittent faults on live wires. Dr. Furse teaches electromagnetics, wireless communication, computational electromagnetics, microwave engineering, and antenna design. Dr. Furse was the Professor of the Year in the College of Engineering at Utah State University for the year 2000, and Faculty Employee of the year 2002. She is the chair of the IEEE Antennas and Propagation Society Education Committee, and associate editor of the IEEE Transactions on Antennas and Propagation.

2006 INSTITUTIONAL MEMBERS

AUSTRALIAN DEFENCE LIBRARY
Northcott Drive
Campbell, A.C.T. 2600 AUSTRALIA

BEIJING BOOK COMPANY, INC
701 E Lindon Ave.
Linden, NJ 07036-2495

BRITISH LIBRARY
Boston SPA, Wetherby
West Yorkshire, UK LS23 7BQ

DARMSTADT U. OF TECHNOLOGY
Schlossgartenstrasse 8
Darmstadt, Hessen
GERMANY D-64289

DARTMOUTH COLL-FELDBERG LIB
6193 Murdough Center
Hanover, NH 03755-3560

DEFENCE RESEARCH ESTAB. LIB.
3701 Carling Avenue
Ottawa, ON, K1A 0Z4 CANADA

DLR-STANDORTBIBLIOTEK
Muenchnerstrasse 20
Wessling, Germany 82234

DPS/LIBRARY (EABV)
Alion Science & Technology
185 Admiral Cochrane Drive
Annapolis, MD 214017307

DSTO-DSTORL EDINBURGH
Jets AU/33851-99, PO Box 562
Milsons Point, NSW
AUSTRALIA 1565

DTIC-OCP/LIBRARY
8725 John J. Kingman Rd. Ste 0944
Ft. Belvoir, VA 22060-6218

ELLEDIEMME SRL
Via Baccina 30
Roma, Italy 00184

ELSEVIER
Bibliographic Databases
PO Box 2227
Amsterdam, Netherlands 1000 CE

ENGINEERING INFORMATION, INC
PO Box 543
Amsterdam, Netherlands 1000 Am

ETSE TELECOMUNICACION
Biblioteca, Campus Lagoas
Vigo, 36200 SPAIN

FGAN-FHR
Neuenahrerstrasse 20
Wachtberg, Germany 53343

FLORIDA INTERNATIONAL UNIV.
ECE Dept./EAS-3983
10555 W. Flagler St
Miami, FL 33174

GEORGIA TECH LIBRARY
225 North Avenue, NW
Atlanta, GA 30332-0001

HRL LABS, RESEARCH LIBRARY
3011 Malibu Canyon
Malibu, CA 90265

IEE INSPEC/Acquisitions Section
Michael Faraday House
6 Hills Way
Stevenage, Herts UK SG1 2AY

IND CANTABRIA
PO Box 830470
Birmingham, AL 35283

INSTITUTE FOR SCIENTIFIC INFO.
Publication Processing Dept.
3501 Market St.
Philadelphia, PA 19104-3302

LIBRARY of CONGRESS
Reg. Of Copyrights
Attn: 40T Deposits
Washington DC, 20559

LINDA HALL LIBRARY
5109 Cherry Street
Kansas City, MO 64110-2498

MISSISSIPPI STATE UNIV LIBRARY
PO Box 9570
Mississippi State, MS 39762

MIT LINCOLN LABORATORY
Periodicals Library
244 Wood Street
Lexington, MA 02420

NA KANSAI KINOKUNNA CO.
Attn: M. MIYOSHI
PO Box 36 (NDLA KANSAI)
Hongo, Tokyo, JAPAN 113-8688

NATL. CTR. FOR HIGH-
PERFORMANCE COMPUTING LIB.
PO Box 117-00930
Taipei City, Taiwan (ROC) 10699

NATL. GROUND INTELL. CENTER
2055 Boulders Road
Charlottesville, VA 22911-8318

NAVAL POSTGRADUATE SCHOOL
Attn: J. Rozdal/411 Dyer Rd./ Rm 111
Monterey, CA 93943-5101

NAVAL RESEARCH LABORATORY
C. Office, 4555 Overlook Avenue, SW
Washington, DC 20375

OHIO STATE UNIVERSITY
1320 Kinnear Road
Columbus, OH 43212

OVIEDO LIBRARY
PO BOX 830679
Birmingham, AL 35283

PAIKNAM ACAD. INFO CTR LIB.
Hanyang U/17 Haengdang-Dong
Seongdong-ki, Seoul, S Korea 133-
791

PENN STATE UNIVERSITY
126 Paterno Library
University Park, PA 16802-1808

PHILIPS RESEARCH LAB
Cross Oak Lane, Stella Cox, Salfords
Red Hill, UK RH1 5HA

RENTON TECH LIBRARY/BOEING
PO BOX 3707
SEATTLE, WA 98124-2207

SOUTHWEST RESEARCH INST.
6220 Culebra Road
San Antonio, TX 78238

SWEDISH DEFENCE RES.
AGENCY (FOI)
PO Box 1165
Linkoping, Sweden S-58111

SWETS INFORMATION SERVICES
160 Ninth Avenue, Suite A
Runnemede, NJ 08078

SYRACUSE UNIVERSITY
EECS, 121 Link Hall
Syracuse, NY 13244

TECHNISCHE UNIV. DELFT
Mekelweg 4, Delft, Holland, 2628 CD
NETHERLANDS

TIB & UNIV. BIB. HANNOVER
DE/5100/G1/0001
Welfengarten 1B
Hannover, GERMANY 30167

TOKYO KOKA UNIVERSITY
1404-1 Katakura-Cho
Hachioji, Tokyo, JAPAN 192-0914

UNIV OF CENTRAL FLORIDA LIB.
4000 Central Florida Boulevard
Orlando, FL 32816-8005

UNIV OF COLORADO LIBRARY
Campus Box 184
Boulder, CO 80309-0184

UNIVERSITY OF MISSISSIPPI
John Davis Williams Library
PO Box 1848
University, MS 38677-1848

UNIV OF MISSOURI-ROLLA LIB.
1870 Miner Circle
Rolla, MO 65409-0001

USAE ENG. RES. & DEV. CENTER
Attn: Library/Journals
72 Lyme Road
Hanover, NH 03755-1290

USP POLI
Av: Elmira Martins Moreira, 455
Jacarei, Sao Paulo, Brazil 12306-730

ACES COPYRIGHT FORM

This form is intended for original, previously unpublished manuscripts submitted to ACES periodicals and conference publications. The signed form, appropriately completed, MUST ACCOMPANY any paper in order to be published by ACES. PLEASE READ REVERSE SIDE OF THIS FORM FOR FURTHER DETAILS.

TITLE OF PAPER:

RETURN FORM TO:

Dr. Atef Z. Elsherbeni
University of Mississippi
Dept. of Electrical Engineering
Anderson Hall Box 13
University, MS 38677 USA

AUTHORS(S)

PUBLICATION TITLE/DATE:

PART A - COPYRIGHT TRANSFER FORM

(NOTE: Company or other forms may not be substituted for this form. U.S. Government employees whose work is not subject to copyright may so certify by signing Part B below. Authors whose work is subject to Crown Copyright may sign Part C overleaf).

The undersigned, desiring to publish the above paper in a publication of ACES, hereby transfer their copyrights in the above paper to The Applied Computational Electromagnetics Society (ACES). The undersigned hereby represents and warrants that the paper is original and that he/she is the author of the paper or otherwise has the power and authority to make and execute this assignment.

Returned Rights: In return for these rights, ACES hereby grants to the above authors, and the employers for whom the work was performed, royalty-free permission to:

1. Retain all proprietary rights other than copyright, such as patent rights.
2. Reuse all or portions of the above paper in other works.

3. Reproduce, or have reproduced, the above paper for the author's personal use or for internal company use provided that (a) the source and ACES copyright are indicated, (b) the copies are not used in a way that implies ACES endorsement of a product or service of an employer, and (c) the copies per se are not offered for sale.

4. Make limited distribution of all or portions of the above paper prior to publication.

5. In the case of work performed under U.S. Government contract, ACES grants the U.S. Government royalty-free permission to reproduce all or portions of the above paper, and to authorize others to do so, for U.S. Government purposes only.

ACES Obligations: In exercising its rights under copyright, ACES will make all reasonable efforts to act in the interests of the authors and employers as well as in its own interest. In particular, ACES REQUIRES that:

1. The consent of the first-named author be sought as a condition in granting re-publication permission to others.
2. The consent of the undersigned employer be obtained as a condition in granting permission to others to reuse all or portions of the paper for promotion or marketing purposes.

In the event the above paper is not accepted and published by ACES or is withdrawn by the author(s) before acceptance by ACES, this agreement becomes null and void.

AUTHORIZED SIGNATURE

TITLE (IF NOT AUTHOR)

EMPLOYER FOR WHOM WORK WAS PERFORMED

DATE FORM SIGNED

Part B - U.S. GOVERNMENT EMPLOYEE CERTIFICATION

(NOTE: if your work was performed under Government contract but you are not a Government employee, sign transfer form above and see item 5 under Returned Rights).

This certifies that all authors of the above paper are employees of the U.S. Government and performed this work as part of their employment and that the paper is therefor not subject to U.S. copyright protection.

AUTHORIZED SIGNATURE

TITLE (IF NOT AUTHOR)

NAME OF GOVERNMENT ORGANIZATION

DATE FORM SIGNED

PART C - CROWN COPYRIGHT

(NOTE: ACES recognizes and will honor Crown Copyright as it does U.S. Copyright. It is understood that, in asserting Crown Copyright, ACES in no way diminishes its rights as publisher. Sign only if ALL authors are subject to Crown Copyright).

This certifies that all authors of the above Paper are subject to Crown Copyright. (Appropriate documentation and instructions regarding form of Crown Copyright notice may be attached).

AUTHORIZED SIGNATURE

TITLE OF SIGNEE

NAME OF GOVERNMENT BRANCH

DATE FORM SIGNED

Information to Authors

ACES POLICY

ACES distributes its technical publications throughout the world, and it may be necessary to translate and abstract its publications, and articles contained therein, for inclusion in various compendiums and similar publications, etc. When an article is submitted for publication by ACES, acceptance of the article implies that ACES has the rights to do all of the things it normally does with such an article.

In connection with its publishing activities, it is the policy of ACES to own the copyrights in its technical publications, and to the contributions contained therein, in order to protect the interests of ACES, its authors and their employers, and at the same time to facilitate the appropriate re-use of this material by others.

The new United States copyright law requires that the transfer of copyrights in each contribution from the author to ACES be confirmed in writing. It is therefore necessary that you execute either Part A-Copyright Transfer Form or Part B-U.S. Government Employee Certification or Part C-Crown Copyright on this sheet and return it to the Managing Editor (or person who supplied this sheet) as promptly as possible.

CLEARANCE OF PAPERS

ACES must of necessity assume that materials presented at its meetings or submitted to its publications is properly available for general dissemination to the audiences these activities are organized to serve. It is the responsibility of the authors, not ACES, to determine whether disclosure of their material requires the prior consent of other parties and if so, to obtain it. Furthermore, ACES must assume that, if an author uses within his/her article previously published and/or copyrighted material that permission has been obtained for such use and that any required credit lines, copyright notices, etc. are duly noted.

AUTHOR/COMPANY RIGHTS

If you are employed and you prepared your paper as a part of your job, the rights to your paper initially rest with your employer. In that case, when you sign the copyright form, we assume you are authorized to do so by your employer and that your employer has consented to all of the terms and conditions of this form. If not, it should be signed by someone so authorized.

NOTE RE RETURNED RIGHTS: Just as ACES now requires a signed copyright transfer form in order to do "business as usual", it is the intent of this form to return rights to the author and employer so that they too may do "business as usual". If further clarification is required, please contact: The Managing Editor, R. W. Adler, Naval Postgraduate School, Code EC/AB, Monterey, CA, 93943, USA (408)656-2352.

Please note that, although authors are permitted to re-use all or portions of their ACES copyrighted material in other works, this does not include granting third party requests for reprinting, republishing, or other types of re-use.

JOINT AUTHORSHIP

For jointly authored papers, only one signature is required, but we assume all authors have been advised and have consented to the terms of this form.

U.S. GOVERNMENT EMPLOYEES

Authors who are U.S. Government employees are not required to sign the Copyright Transfer Form (Part A), but any co-authors outside the Government are.

Part B of the form is to be used instead of Part A only if all authors are U.S. Government employees and prepared the paper as part of their job.

NOTE RE GOVERNMENT CONTRACT WORK: Authors whose work was performed under a U.S. Government contract but who are not Government employees are required so sign Part A-Copyright Transfer Form. However, item 5 of the form returns reproduction rights to the U. S. Government when required, even though ACES copyright policy is in effect with respect to the reuse of material by the general public.

January 2002

INFORMATION FOR AUTHORS

PUBLICATION CRITERIA

Each paper is required to manifest some relation to applied computational electromagnetics. **Papers may address general issues in applied computational electromagnetics, or they may focus on specific applications, techniques, codes, or computational issues.** While the following list is not exhaustive, each paper will generally relate to at least one of these areas:

- 1. Code validation.** This is done using internal checks or experimental, analytical or other computational data. Measured data of potential utility to code validation efforts will also be considered for publication.
- 2. Code performance analysis.** This usually involves identification of numerical accuracy or other limitations, solution convergence, numerical and physical modeling error, and parameter tradeoffs. However, it is also permissible to address issues such as ease-of-use, set-up time, run time, special outputs, or other special features.
- 3. Computational studies of basic physics.** This involves using a code, algorithm, or computational technique to simulate reality in such a way that better, or new physical insight or understanding, is achieved.
- 4. New computational techniques,** or new applications for existing computational techniques or codes.
- 5. “Tricks of the trade”** in selecting and applying codes and techniques.
- 6. New codes, algorithms, code enhancement, and code fixes.** This category is self-explanatory, but includes significant changes to existing codes, such as applicability extensions, algorithm optimization, problem correction, limitation removal, or other performance improvement. **Note: Code (or algorithm) capability descriptions are not acceptable, unless they contain sufficient technical material to justify consideration.**
- 7. Code input/output issues.** This normally involves innovations in input (such as input geometry standardization, automatic mesh generation, or computer-aided design) or in output (whether it be tabular, graphical, statistical, Fourier-transformed, or otherwise signal-processed). Material dealing with input/output database management, output interpretation, or other input/output issues will also be considered for publication.
- 8. Computer hardware issues.** This is the category for analysis of hardware capabilities and limitations of various types of electromagnetics computational requirements. Vector and parallel computational techniques and implementation are of particular interest.

Applications of interest include, but are not limited to, antennas (and their electromagnetic environments), networks, static fields, radar cross section, shielding, radiation hazards, biological effects, electromagnetic pulse (EMP), electromagnetic interference (EMI), electromagnetic compatibility (EMC), power transmission, charge transport, dielectric, magnetic and nonlinear materials, microwave components, MEMS technology, MMIC technology, remote sensing and geometrical and physical optics, radar and communications systems, fiber optics, plasmas, particle accelerators, generators and motors, electromagnetic wave propagation, non-destructive evaluation, eddy currents, and inverse scattering.

Techniques of interest include frequency-domain and time-domain techniques, integral equation and differential equation techniques, diffraction theories, physical optics, moment methods, finite differences and finite element techniques, modal expansions, perturbation methods, and hybrid methods. This list is not exhaustive.

A unique feature of the Journal is the publication of unsuccessful efforts in applied computational electromagnetics. Publication of such material provides a means to discuss problem areas in electromagnetic modeling. Material representing an unsuccessful application or negative results in computational electromagnetics will be considered for publication only if a reasonable expectation of success (and a reasonable effort) are reflected. Moreover, such material must represent a problem area of potential interest to the ACES membership.

Where possible and appropriate, authors are required to provide statements of quantitative accuracy for measured and/or computed data. This issue is discussed in “Accuracy & Publication: Requiring, quantitative accuracy statements to accompany data,” by E. K. Miller, *ACES Newsletter*, Vol. 9, No. 3, pp. 23-29, 1994, ISBN 1056-9170.

EDITORIAL REVIEW

In order to ensure an appropriate level of quality control, papers are peer reviewed. They are reviewed both for technical correctness and for adherence to the listed guidelines regarding information content.

JOURNAL CAMERA-READY SUBMISSION DATES

March issue	deadline 8 January
July issue	deadline 20 May
November issue	deadline 20 September

Uploading an acceptable camera-ready article after the deadlines will result in a delay in publishing this article.

STYLE FOR CAMERA-READY COPY

The ACES Journal is flexible, within reason, in regard to style. However, certain requirements are in effect:

1. The paper title should NOT be placed on a separate page. The title, author(s), abstract, and (space permitting) beginning of the paper itself should all be on the first page. The title, author(s), and author affiliations should be centered (center-justified) on the first page.
2. An abstract is REQUIRED. The abstract should be a brief summary of the work described in the paper. It should state the computer codes, computational techniques, and applications discussed in the paper (as applicable) and should otherwise be usable by technical abstracting and indexing services.
3. Either British English or American English spellings may be used, provided that each word is spelled consistently throughout the paper.
4. Any commonly-accepted format for referencing is permitted, provided that internal consistency of format is maintained. As a guideline for authors who have no other preference, we recommend that references be given by author(s) name and year in the body of the paper (with alphabetical listing of all references at the end of the paper). Titles of Journals, monographs, and similar publications should be in italic font or should be underlined. Titles of papers or articles should be in quotation marks.
5. Internal consistency shall also be maintained for other elements of style, such as equation numbering. As a guideline for authors who have no other preference, we suggest that equation numbers be placed in parentheses at the right column margin.
6. The intent and meaning of all text must be clear. For authors who are NOT masters of the English language, the ACES Editorial Staff will provide assistance with grammar (subject to clarity of intent and meaning).
7. Unused space should be minimized. Sections and subsections should not normally begin on a new page.

PAPER FORMAT

The preferred format for initial submission and camera-ready manuscripts is 12 point Times Roman font, single line spacing and double column format, similar to that used here, with top, bottom, left, and right 1 inch margins. Manuscripts should be prepared on standard 8.5x11 inch paper.

Only camera-ready electronic files are accepted for publication. The term **“camera-ready”** means that the material is neat, legible, and reproducible. Full details can be found on ACES site, Journal section.

ACES reserves the right to edit any uploaded material, however, this is not generally done. It is the author(s)

responsibility to provide acceptable camera-ready pdf files. Incompatible or incomplete pdf files will not be processed, and authors will be requested to re-upload a revised acceptable version.

SUBMITTAL PROCEDURE

All submissions should be uploaded to ACES server through ACES web site (<http://aces.ee.olemiss.edu>) by using the upload button, journal section. Only pdf files are accepted for submission. The file size should not be larger than 5MB, otherwise permission from the Editor-in-Chief should be obtained first. The Editor-in-Chief will acknowledge the electronic submission after the upload process is successfully completed.

COPYRIGHTS AND RELEASES

Each primary author must sign a copyright form and obtain a release from his/her organization vesting the copyright with ACES. Copyright forms are available at ACES, web site (<http://aces.ee.olemiss.edu>). To shorten the review process time, the executed copyright form should be forwarded to the Editor-in-Chief immediately after the completion of the upload (electronic submission) process. Both the author and his/her organization are allowed to use the copyrighted material freely for their own private purposes.

Permission is granted to quote short passages and reproduce figures and tables from and ACES Journal issue provided the source is cited. Copies of ACES Journal articles may be made in accordance with usage permitted by Sections 107 or 108 of the U.S. Copyright Law. This consent does not extend to other kinds of copying, such as for general distribution, for advertising or promotional purposes, for creating new collective works, or for resale. The reproduction of multiple copies and the use of articles or extracts for commercial purposes require the consent of the author and specific permission from ACES. Institutional members are allowed to copy any ACES Journal issue for their internal distribution only.

PUBLICATION CHARGES

ACES members are allowed 12 printed pages per paper without charge; non-members are allowed 8 printed pages per paper without charge. Mandatory page charges of \$75 a page apply to all pages in excess of 12 for members or 8 for non-members. Voluntary page charges are requested for the free (12 or 8) pages, but are NOT mandatory or required for publication. A priority courtesy guideline, which favors members, applies to paper backlogs. Authors are entitled to 15 free reprints of their articles and must request these from the Managing Editor. Additional reprints are available to authors, and reprints available to non-authors, for a nominal fee.

ACES Journal is abstracted in INSPEC, in Engineering Index, and in DTIC.